

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA\_U\DATA\VU081418\  
 Data File : VU026111.D  
 Acq On : 14 Aug 2018 19:32  
 Operator : MD/SY  
 Sample : J4451-17  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 A4ZK5

Quant Time: Aug 14 19:51:56 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM080918WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Aug 14 02:18:47 2018  
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	254716	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	234737	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	96407	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	72814	39.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.22%
7) Chloroethane-d5	1.68	69	66646	45.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.30%
11) 1,1-Dichloroethene-d2	2.27	63	113755	32.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.30%
21) 2-Butanone-d5	4.18	46	146194	94.21	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.21%
24) Chloroform-d	4.65	84	187614	47.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.04%
26) 1,2-Dichloroethane-d4	5.31	65	128572	48.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.42%
32) Benzene-d6	5.35	84	351576	48.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.46%
36) 1,2-Dichloropropane-d6	6.33	67	116005	49.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.36%
41) Toluene-d8	7.57	98	312222	44.77	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.54%
43) trans-1,3-Dichloropropene-	7.85	79	53999	45.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.88%
47) 2-Hexanone-d5	8.31	63	99163	92.57	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.57%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	167359	48.52	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.04%
64) 1,2-Dichlorobenzene-d4	11.86	152	122339	51.48	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.96%


Target Compounds						Qvalue
13) Acetone	2.32	43	5033	5.221	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA\_U\DATA\VU081418\  
 Data File : VU026111.D  
 Acq On : 14 Aug 2018 19:32  
 Operator : MD/SY  
 Sample : J4451-17  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampled :  
 A4ZK5

Quant Time: Aug 14 19:51:56 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM080918WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Aug 14 02:18:47 2018  
 Response via : Initial Calibration

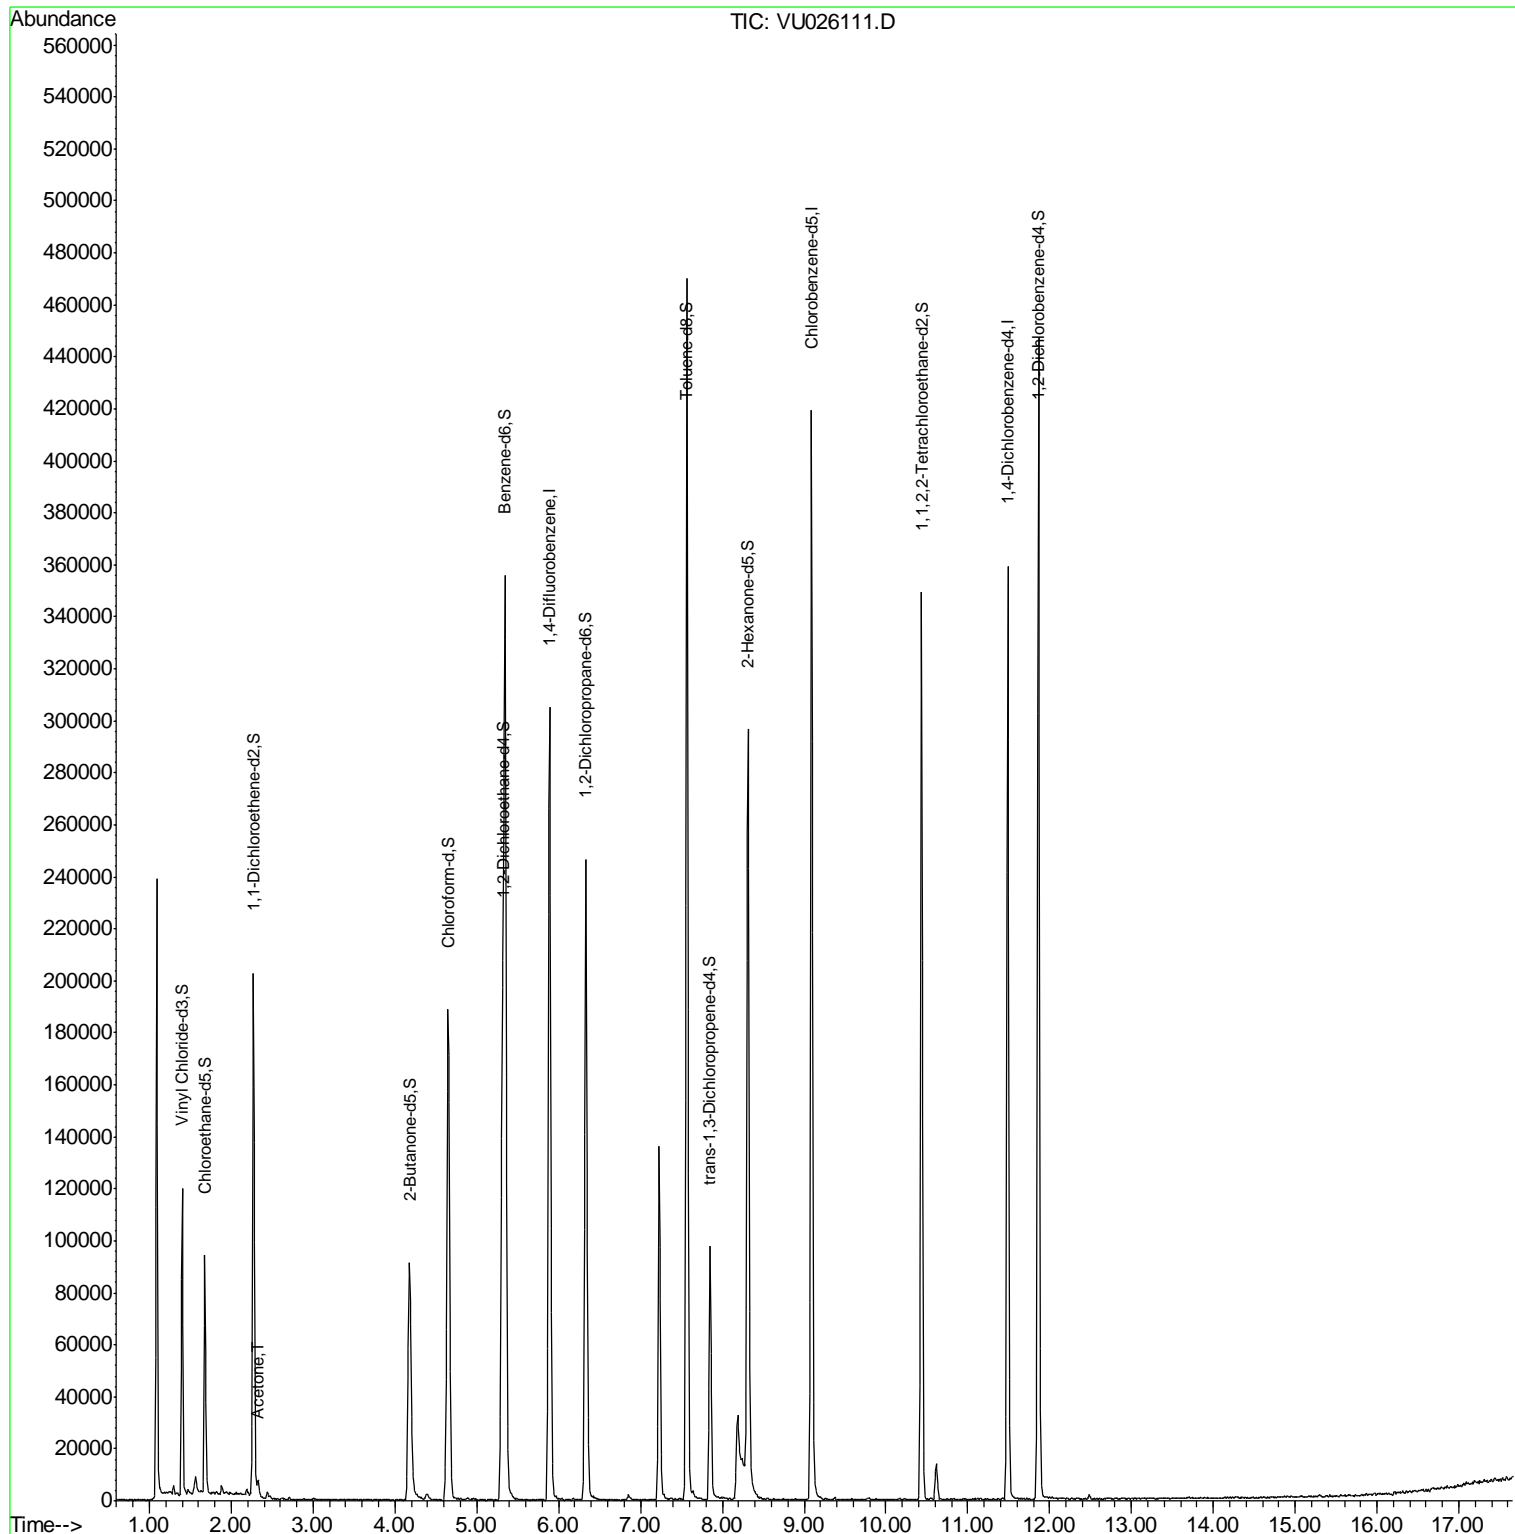

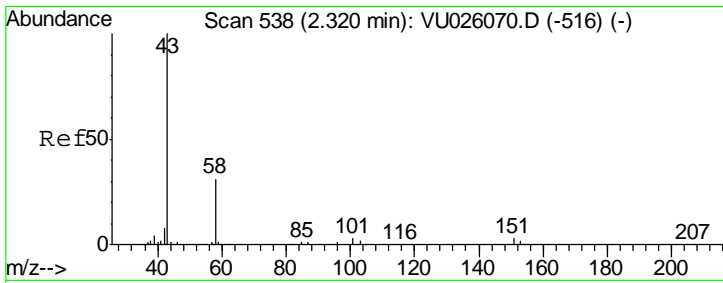

#13  
 Acetone  
 Concen: 5.221 ug/L  
 RT: 2.32 min Scan# 539  
 Delta R.T. 0.00 min  
 Lab File: VU026111.D  
 Acq: 14 Aug 2018 19:32

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 A4ZK5

Tgt Ion: 43 Resp: 5033  
 Ion Ratio Lower Upper  
 43 100  
 58 28.7 0.0 61.8

