

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
 Data File : VU026100.D
 Acq On : 14 Aug 2018 14:41
 Operator : MD/SY
 Sample : J4451-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZJ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.670	23	25	27	rVB	222	94	0.01%	0.001%
2	0.693	27	32	34	rBV2	191	167	0.02%	0.002%
3	0.712	35	38	44	rVB	302	267	0.02%	0.003%
4	0.741	44	47	49	rBV	307	216	0.02%	0.003%
5	0.751	49	50	55	rVB	225	101	0.01%	0.001%
6	0.773	55	57	59	rVB	78	33	0.00%	0.000%
7	0.789	59	62	66	rBV3	412	362	0.03%	0.004%
8	0.838	72	77	79	rBV	309	266	0.02%	0.003%
9	0.854	79	82	86	rVV2	271	152	0.01%	0.002%
10	0.886	89	92	96	rBV	261	228	0.02%	0.003%
11	0.950	108	112	113	rBV	113	79	0.01%	0.001%
12	0.982	119	122	124	rVB3	358	204	0.02%	0.002%
13	0.998	124	127	128	rBV2	166	109	0.01%	0.001%
14	1.088	139	155	175	rBV	336986	394830	36.14%	4.663%
15	1.400	245	252	264	rVB	125020	125413	11.48%	1.481%
16	1.677	331	338	354	rVB	95205	128112	11.73%	1.513%
17	2.272	513	523	536	rBV	212858	322821	29.55%	3.812%
18	3.378	864	867	869	rBV2	503	327	0.03%	0.004%
19	3.458	890	892	893	rBV2	280	147	0.01%	0.002%
20	3.564	923	925	927	rVB	152	64	0.01%	0.001%
21	3.603	935	937	940	rVB2	173	99	0.01%	0.001%
22	3.638	945	948	956	rBV2	398	453	0.04%	0.005%
23	3.699	965	967	969	rBV	168	84	0.01%	0.001%
24	3.722	970	974	975	rVV2	282	193	0.02%	0.002%
25	3.751	979	983	985	rBV	399	221	0.02%	0.003%
26	3.879	1020	1023	1033	rVB	240	206	0.02%	0.002%
27	3.921	1033	1036	1037	rBV	208	125	0.01%	0.001%
28	3.953	1043	1046	1048	rBV	57	44	0.00%	0.001%
29	3.982	1052	1055	1059	rVB	355	283	0.03%	0.003%
30	4.008	1060	1063	1068	rVB2	292	246	0.02%	0.003%
31	4.040	1071	1073	1075	rBV	176	56	0.01%	0.001%
32	4.056	1075	1078	1079	rBV	289	128	0.01%	0.002%
33	4.111	1092	1095	1097	rBV2	235	173	0.02%	0.002%
34	4.175	1101	1115	1142	rVV	92642	237426	21.73%	2.804%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
 Data File : VU026100.D
 Acq On : 14 Aug 2018 14:41
 Operator : MD/SY
 Sample : J4451-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZJ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

35	4.439	1196	1197	1198	rBV	206	51	0.00%	0.001%
36	4.452	1198	1201	1204	rVV3	334	234	0.02%	0.003%
37	4.474	1204	1208	1210	rVB	478	333	0.03%	0.004%
38	4.493	1210	1214	1219	rBV	419	443	0.04%	0.005%
39	4.590	1242	1244	1245	rVB	246	85	0.01%	0.001%
40	4.651	1245	1263	1291	rBV	190845	449028	41.10%	5.303%
41	4.857	1325	1327	1329	rVB2	380	175	0.02%	0.002%
42	4.889	1329	1337	1339	rBV4	774	1048	0.10%	0.012%
43	5.034	1379	1382	1384	rBV	269	141	0.01%	0.002%
44	5.098	1399	1402	1405	rVB	266	130	0.01%	0.002%
45	5.117	1405	1408	1412	rBV	316	286	0.03%	0.003%
46	5.140	1412	1415	1417	rVV2	441	303	0.03%	0.004%
47	5.165	1421	1423	1426	rVB3	284	153	0.01%	0.002%
48	5.220	1438	1440	1444	rBV	325	220	0.02%	0.003%
49	5.243	1445	1447	1449	rVB	155	64	0.01%	0.001%
50	5.342	1453	1478	1507	rBV2	364977	1092438	100.00%	12.901%
51	5.542	1537	1540	1542	rBV2	492	290	0.03%	0.003%
52	5.612	1560	1562	1564	rBV	48	28	0.00%	0.000%
53	5.628	1564	1567	1569	rBV	433	262	0.02%	0.003%
54	5.718	1592	1595	1598	rVB2	196	124	0.01%	0.001%
55	5.747	1600	1604	1606	rBV3	337	218	0.02%	0.003%
56	5.789	1615	1617	1619	rBV	215	105	0.01%	0.001%
57	5.815	1623	1625	1628	rVB	239	127	0.01%	0.001%
58	5.837	1629	1632	1633	rBV	170	93	0.01%	0.001%
59	5.889	1634	1648	1673	rVV	309537	602103	55.12%	7.110%
60	6.169	1730	1735	1737	rBV2	336	248	0.02%	0.003%
61	6.188	1737	1741	1742	rBV3	402	291	0.03%	0.003%
62	6.226	1748	1753	1756	rBV	395	364	0.03%	0.004%
63	6.333	1772	1786	1808	rBV	250167	500062	45.77%	5.905%
64	6.606	1868	1871	1874	rBV	348	230	0.02%	0.003%
65	6.622	1874	1876	1881	rBV2	258	208	0.02%	0.002%
66	6.677	1891	1893	1895	rBV	261	141	0.01%	0.002%
67	6.754	1913	1917	1920	rBV2	419	412	0.04%	0.005%
68	6.779	1922	1925	1930	rBV2	373	341	0.03%	0.004%
69	6.831	1939	1941	1943	rBV	205	122	0.01%	0.001%
70	6.853	1943	1948	1951	rBV3	2129	2132	0.20%	0.025%
71	6.992	1990	1991	1995	rVB	322	151	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
 Data File : VU026100.D
 Acq On : 14 Aug 2018 14:41
 Operator : MD/SY
 Sample : J4451-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZJ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

72	7.059	2010	2012	2015	rBV2	351	211	0.02%	0.002%
73	7.075	2015	2017	2019	rBV2	279	179	0.02%	0.002%
74	7.230	2052	2065	2091	rBV	140660	253356	23.19%	2.992%
75	7.500	2147	2149	2150	rBV	220	111	0.01%	0.001%
76	7.567	2157	2170	2190	rBV	486707	843044	77.17%	9.955%
77	7.850	2247	2258	2281	rBV	103200	175867	16.10%	2.077%
78	8.185	2350	2362	2379	rBV	39980	107175	9.81%	1.266%
79	8.313	2393	2402	2430	rVB	289465	503445	46.08%	5.945%
80	8.622	2496	2498	2501	rBV2	353	283	0.03%	0.003%
81	8.702	2520	2523	2524	rBV2	291	166	0.02%	0.002%
82	8.805	2552	2555	2556	rBV	292	181	0.02%	0.002%
83	9.091	2631	2644	2671	rBV	434429	713026	65.27%	8.420%
84	9.377	2728	2733	2735	rBV3	753	711	0.07%	0.008%
85	9.458	2755	2758	2762	rBV	179	112	0.01%	0.001%
86	9.673	2823	2825	2828	rBV	154	90	0.01%	0.001%
87	9.689	2828	2830	2833	rBV2	247	185	0.02%	0.002%
88	9.828	2870	2873	2881	rVB2	256	220	0.02%	0.003%
89	9.860	2881	2883	2884	rBV	207	107	0.01%	0.001%
90	10.165	2974	2978	2979	rBV2	482	326	0.03%	0.004%
91	10.435	3049	3062	3081	rBV	359392	576779	52.80%	6.811%
92	10.612	3107	3117	3131	rVB2	19720	35906	3.29%	0.424%
93	10.889	3198	3203	3208	rBV2	304	368	0.03%	0.004%
94	10.921	3211	3213	3214	rBV	281	149	0.01%	0.002%
95	11.487	3377	3389	3411	rBV	378281	611866	56.01%	7.225%
96	11.718	3460	3461	3468	rVB	595	394	0.04%	0.005%
97	11.770	3473	3477	3480	rBV	440	470	0.04%	0.006%
98	11.863	3494	3506	3530	rBV	484866	776527	71.08%	9.170%


Sum of corrected areas: 8468167

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
Data File : VU026100.D
Acq On : 14 Aug 2018 14:41
Operator : MD/SY
Sample : J4451-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZJ9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

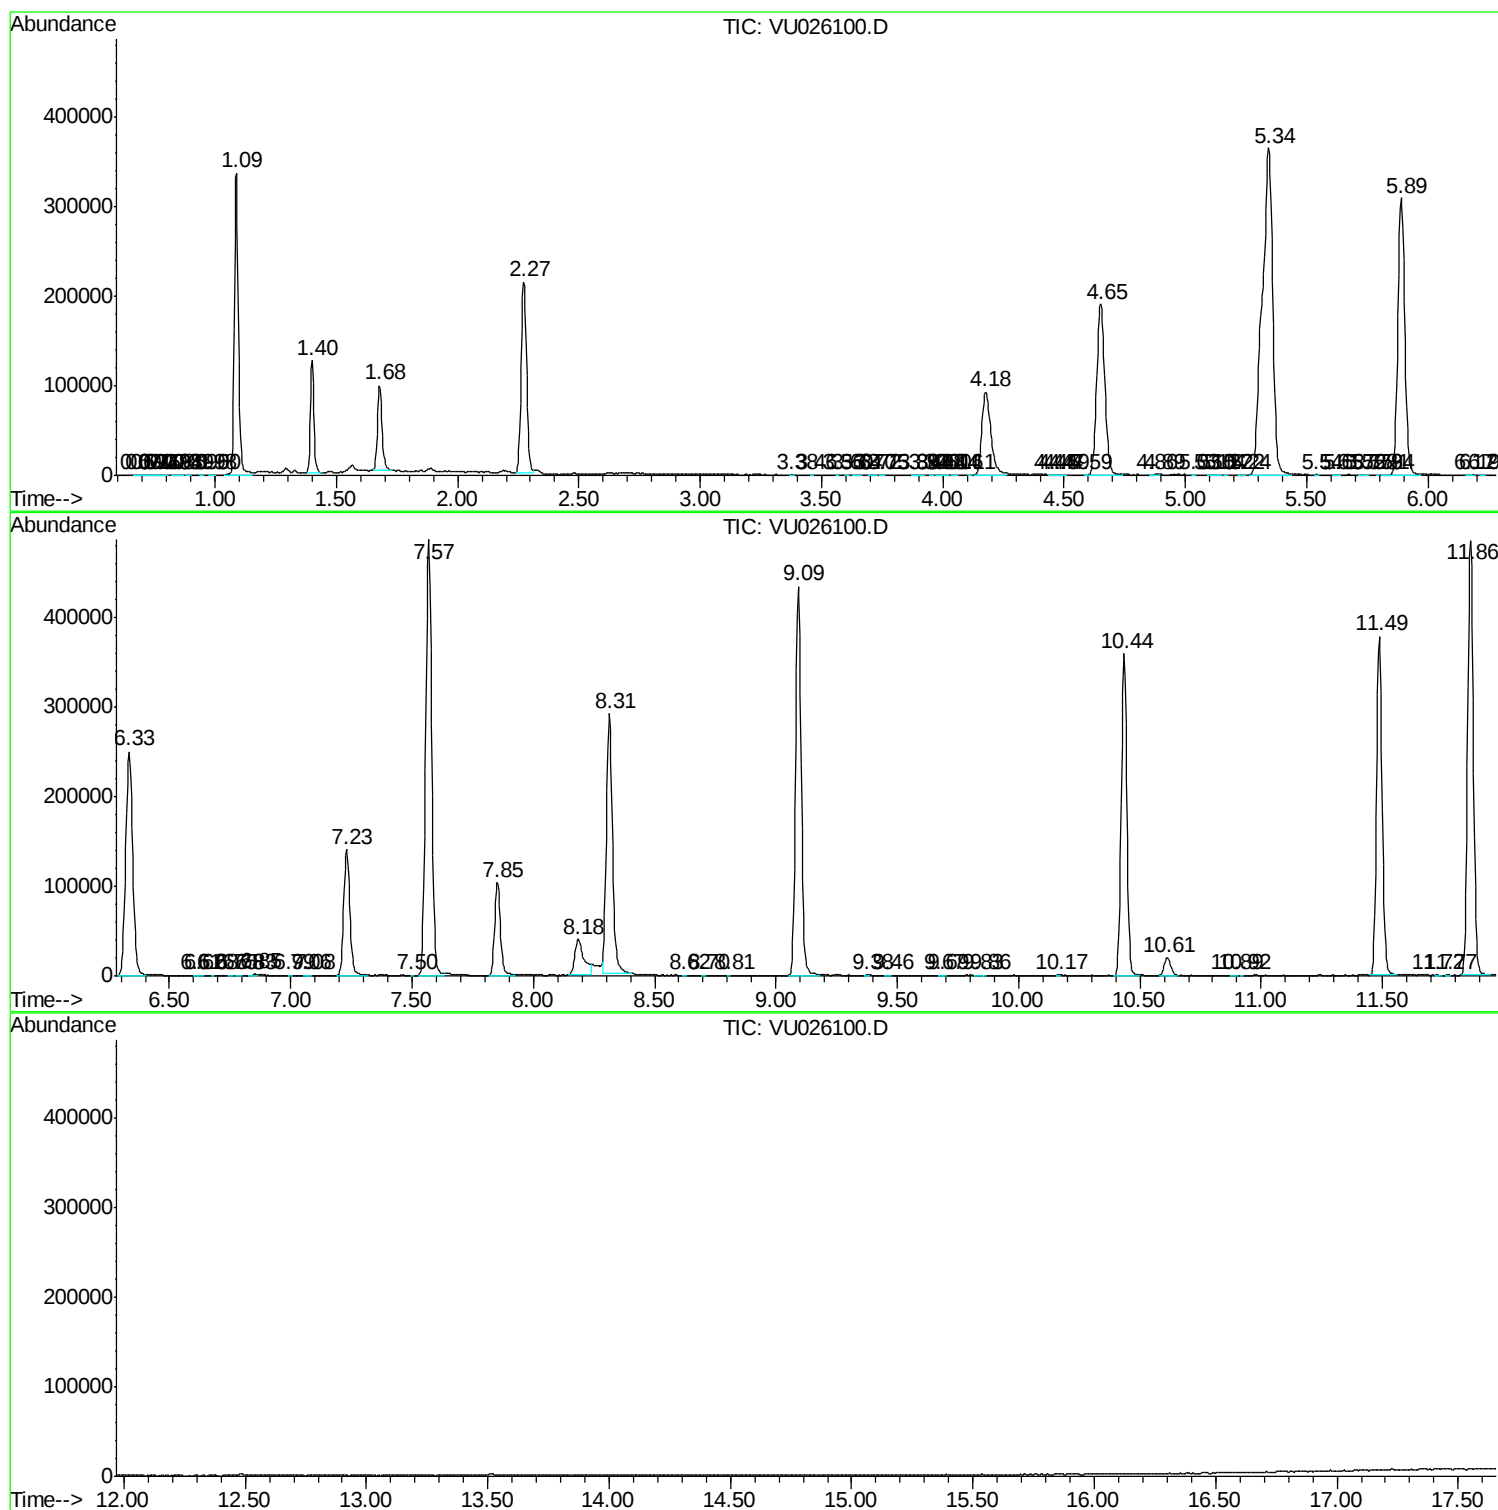

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
Data File : VU026100.D
Acq On : 14 Aug 2018 14:41
Operator : MD/SY
Sample : J4451-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZJ9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
Data File : VU026100.D
Acq On : 14 Aug 2018 14:41
Operator : MD/SY
Sample : J4451-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZJ9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc