


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081418\
Data File : VU026091.D
Acq On : 14 Aug 2018 09:58
Operator : MD/SY
Sample : BFB46
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Title : VOC Analysis
Last Update : Thu Aug 16 01:50:34 2018

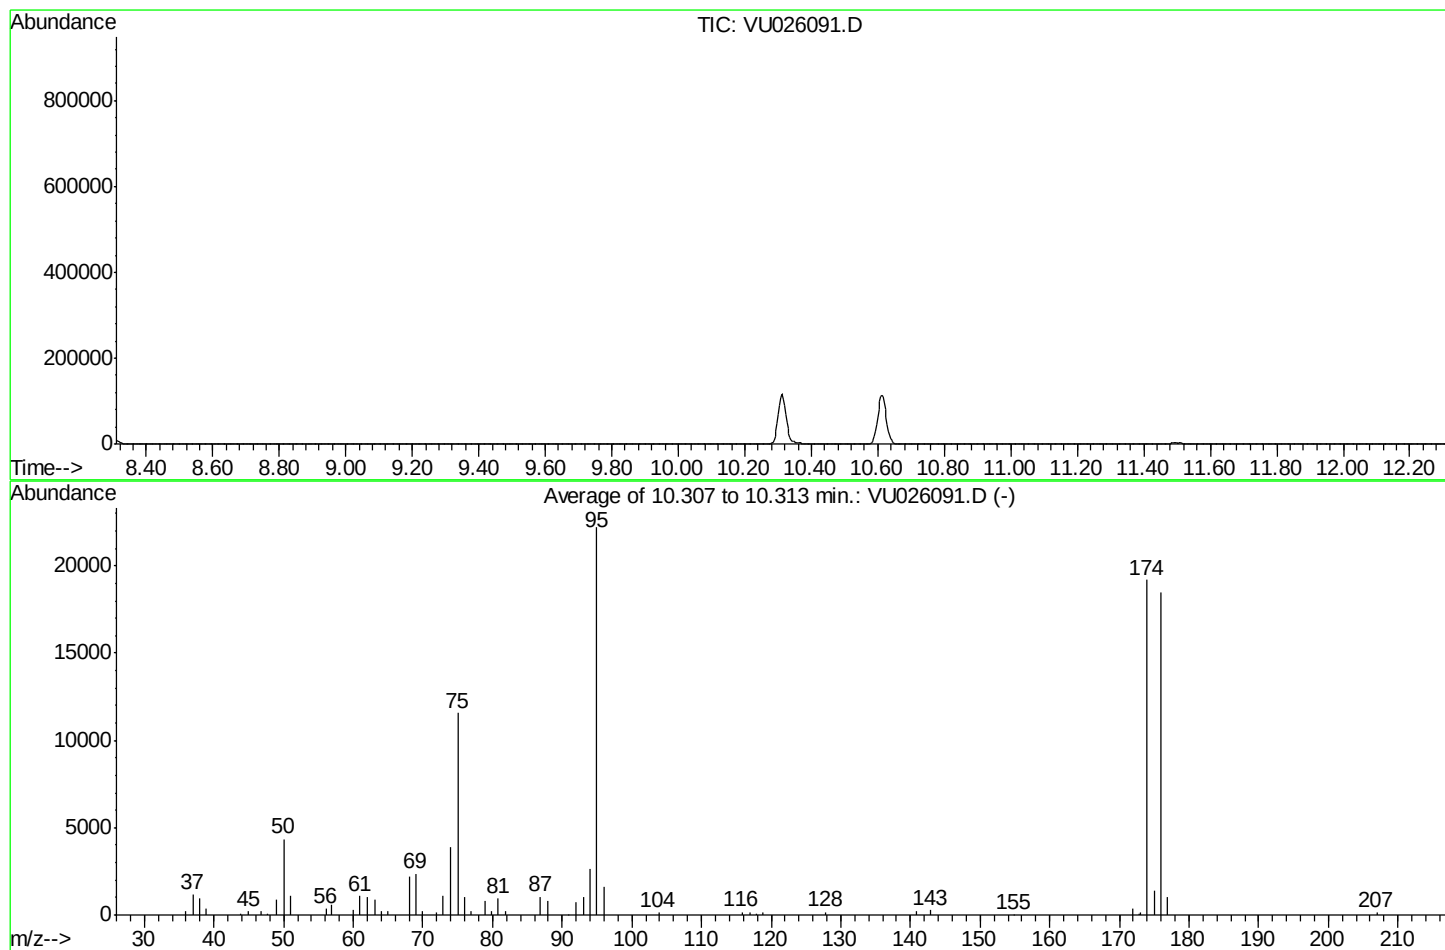

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	4362	PASS
75	95	30	80	52.0	11552	PASS
95	95	100	100	100.0	22208	PASS
96	95	5	9	7.3	1611	PASS
173	174	0.00	2	0.6	117	PASS
174	95	50	120	86.4	19197	PASS
175	174	5	9	7.2	1383	PASS
176	174	95	101	96.2	18474	PASS
177	176	5	9	5.5	1015	PASS

Scan 3011 (10.272 min): VU026091.D
BFB46

m/z	Abundance
39.90	180.0
44.00	423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	217.0
36.90	1090.0
37.90	915.0
39.00	405.0
39.90	155.0
43.90	499.0
45.00	221.0
46.90	247.0
49.00	935.0
50.00	4282.0
51.00	1063.0
56.10	345.0
56.90	545.0
59.90	327.0
61.00	1005.0
62.00	1026.0
63.00	718.0
64.00	152.0
64.90	162.0
68.00	1971.0
69.00	2217.0
70.00	192.0
72.10	150.0
72.90	996.0
74.00	3799.0
75.00	11024.0
76.00	1007.0
76.90	157.0
78.90	753.0
79.90	255.0
80.90	759.0
81.90	218.0
86.90	872.0
87.90	726.0
92.00	777.0
93.00	1045.0
94.00	2374.0
95.00	21480.0
96.00	1472.0
103.90	154.0
115.80	213.0
116.90	136.0
117.90	141.0
118.80	165.0
127.90	140.0
140.70	183.0
142.90	281.0
171.90	341.0
172.80	205.0
174.00	17984.0
174.90	1295.0
176.00	17144.0
176.90	929.0
206.90	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	197.0
36.90	1212.0
37.90	960.0
39.00	372.0
39.90	185.0
43.90	515.0
45.00	232.0
46.80	227.0
47.70	104.0
49.00	903.0
50.00	4479.0
51.00	1165.0
56.10	379.0
57.00	625.0
60.00	293.0
61.00	1104.0
62.00	1076.0
63.00	868.0
63.90	195.0
65.00	259.0
68.00	2293.0
69.00	2397.0
69.90	223.0
72.00	154.0
73.00	1098.0
74.00	4051.0
75.00	11880.0
76.00	1053.0
77.00	229.0
78.90	876.0
79.90	244.0
80.80	970.0
81.90	218.0
86.90	1105.0
88.00	834.0
92.00	745.0
93.00	1025.0
94.00	2734.0
95.00	22912.0
96.00	1677.0
103.90	133.0
115.80	190.0
116.90	166.0
117.90	129.0
118.80	145.0
127.90	171.0
140.80	212.0
142.90	259.0
171.90	340.0
174.00	19680.0
175.00	1397.0
176.00	18920.0
176.90	1033.0
207.00	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	157.0
37.00	1173.0
38.00	922.0
38.90	323.0
39.90	183.0
43.90	531.0
45.00	206.0
46.90	177.0
47.70	129.0
49.00	876.0
50.00	4326.0
51.00	1165.0
56.00	337.0
57.00	642.0
60.00	215.0
61.00	1126.0
62.00	1026.0
63.10	994.0
63.90	211.0
65.00	312.0
68.00	2412.0
69.00	2453.0
69.90	240.0
71.90	135.0
73.00	1105.0
74.00	3906.0
75.00	11754.0
76.00	992.0
76.90	234.0
78.90	907.0
79.90	211.0
80.80	1061.0
81.90	159.0
86.90	1170.0
88.00	931.0
90.80	116.0
92.00	650.0
93.10	918.0
94.00	2761.0
95.00	22232.0
96.00	1686.0
103.80	101.0
115.80	127.0
117.00	187.0
118.90	139.0
127.90	155.0
140.90	252.0
142.90	290.0
154.90	104.0
172.00	329.0
173.10	352.0
174.00	19928.0
175.00	1458.0
176.00	19360.0
177.00	1085.0
207.00	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46