

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081420\
 Data File : VU039871.D
 Acq On : 14 Aug 2020 20:08
 Operator : SY/MD
 Sample : L3517-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 17 05:26:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 17 05:23:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	69053	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	70729	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	33414	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	17823	4.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.60%
7) Chloroethane-d5	1.92	69	19336	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.58	63	25238	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	4.65	46	74888	45.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.32%
24) Chloroform-d	5.09	84	43971	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.72	65	27556	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.75	84	80342	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.70	67	29591	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.91	98	63952	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.19	79	11393	5.16	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.20%
46) 2-Hexanone-d5	8.64	63	57568	48.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.30%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	24987	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	31801	5.56	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.20%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.61	62	5688	1.013	ug/L	96
14) Carbon disulfide	2.80	76	1404	0.109	ug/L #	89
17) Methyl tert-butyl Ether	3.39	73	4624	0.423	ug/L #	85
18) trans-1,2-Dichloroethene	3.37	96	7230	1.577	ug/L	83
22) cis-1,2-Dichloroethene	4.69	96	2178	0.437	ug/L	69
33) Benzene	5.79	78	3061	0.159	ug/L	100
34) Trichloroethene	6.55	95	1287	0.257	ug/L	87
35) Methylcyclohexane	6.70	83	6684	0.837	ug/L #	19
37) 1,2-Dichloropropane	6.70	63	3167	0.619	ug/L #	86
39) cis-1,3-Dichloropropene	7.57	75	779	0.112	ug/L #	62
44) trans-1,3-Dichloropropene	8.18	75	771	0.123	ug/L #	1
48) 2-Hexanone	8.64	43	7290	2.639	ug/L #	65
59) 1,2,3-Trichloropropane	11.81	75	4715	1.277	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081420\
Data File : VU039871.D
Acq On : 14 Aug 2020 20:08
Operator : SY/MD
Sample : L3517-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 17 05:26:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 17 05:23:17 2020
Response via : Initial Calibration

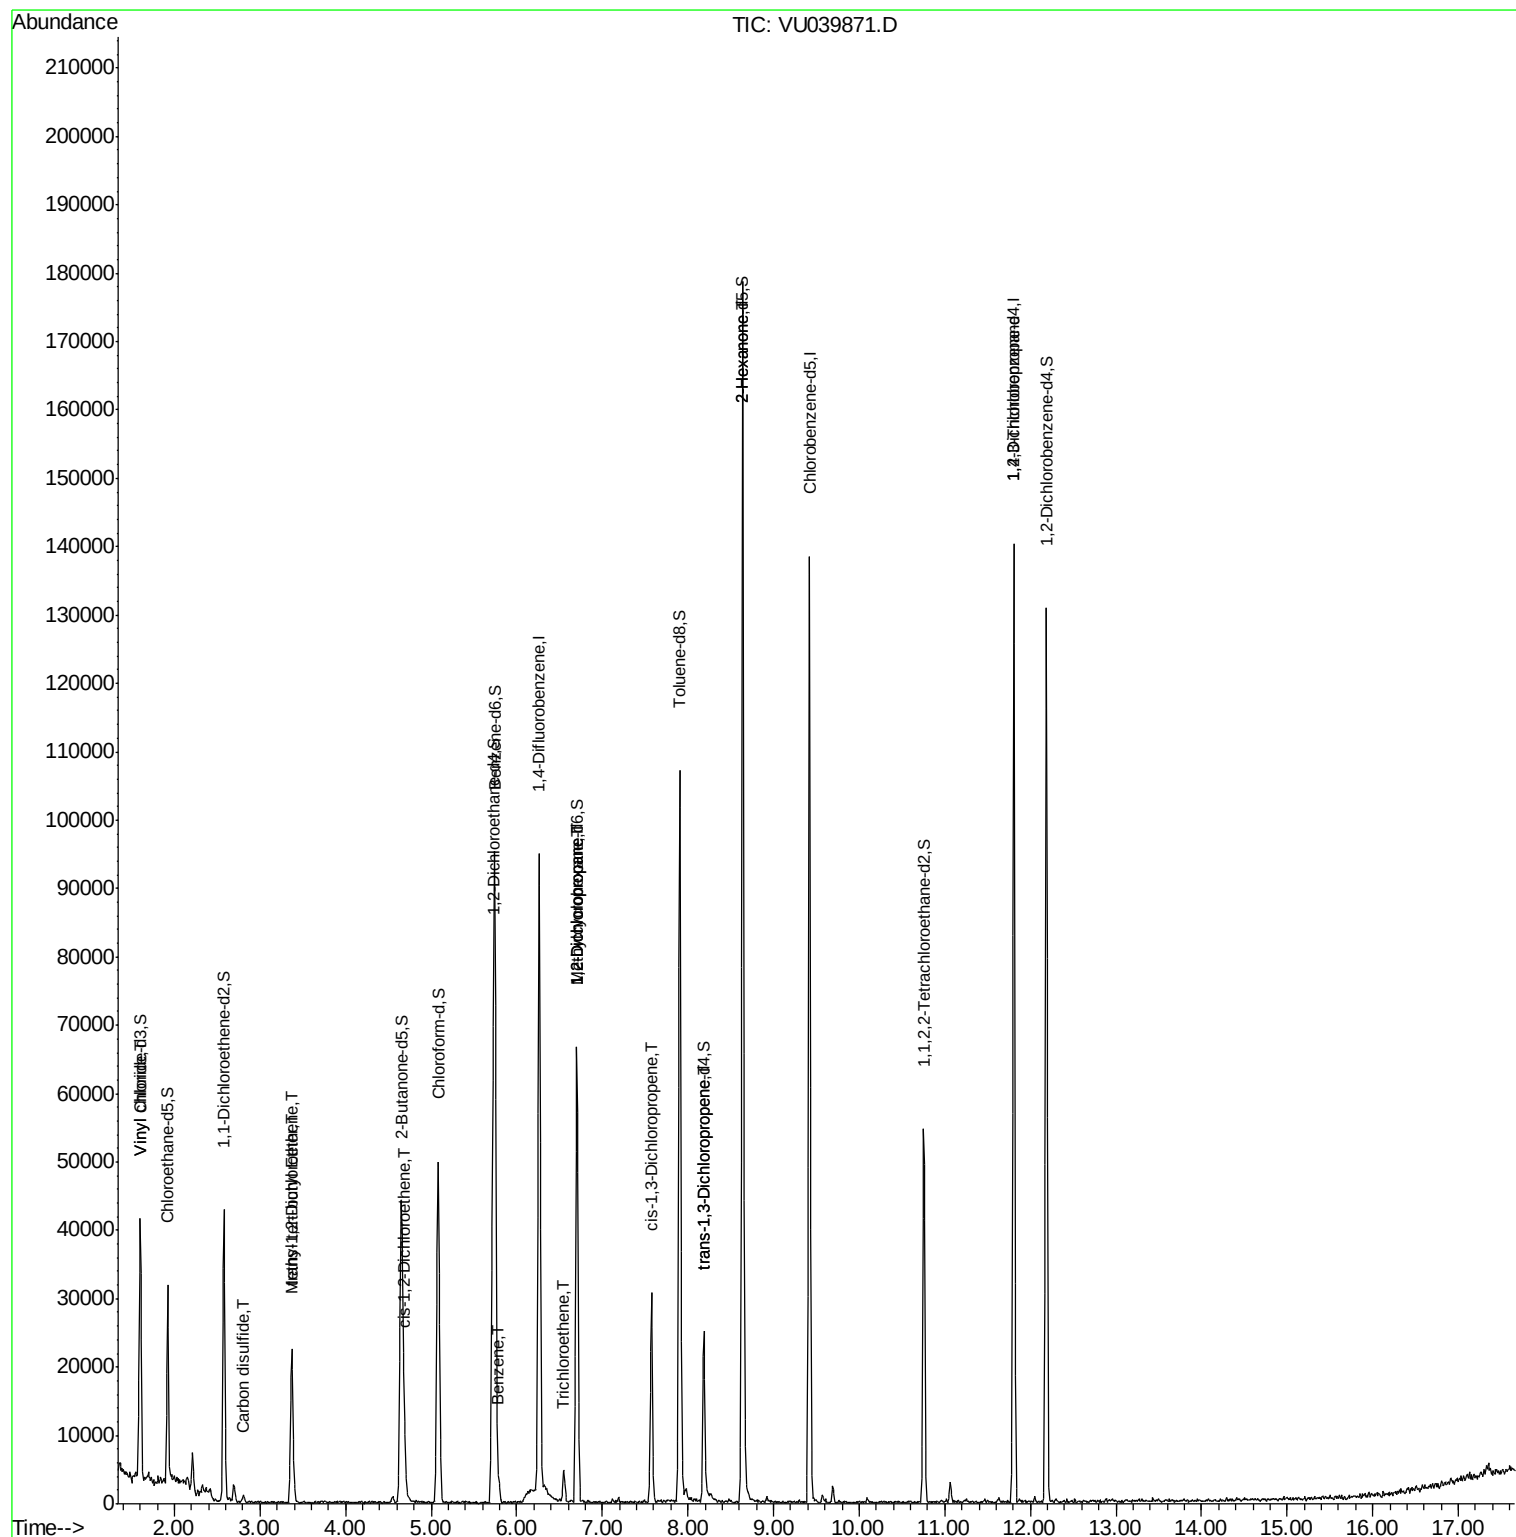

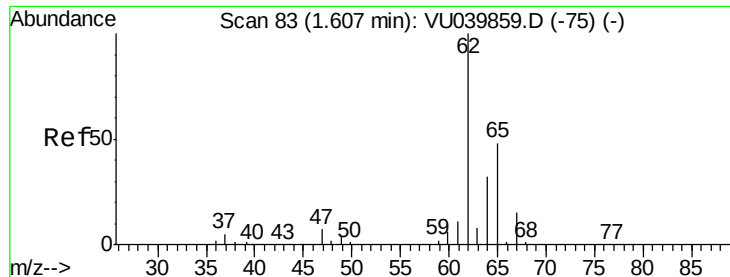

#5

Vinyl chloride

Concen: 1.013 ug/L

RT: 1.61 min Scan# 83

Delta R.T. 0.00 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08

Instrument :

MSVOA_U





ClientSampled :

Tot Ion: 62 Resp: 5688

Ion Ratio Lower Upper

62 100

64 32.2 24.1 44.7

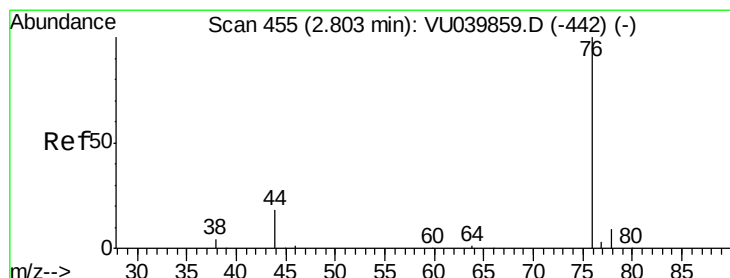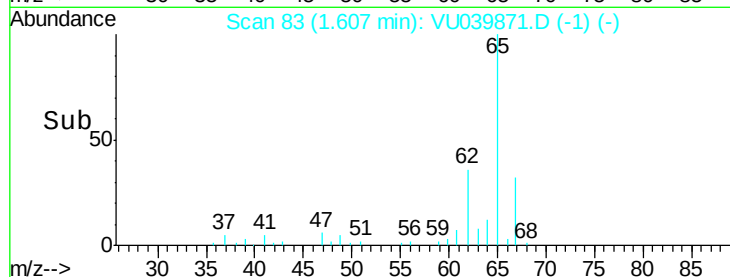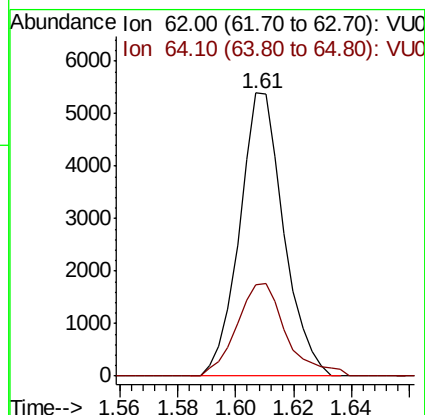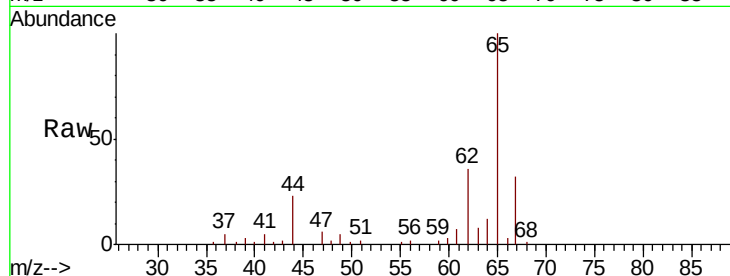

#14

Carbon disulfide

Concen: 0.109 ug/L

RT: 2.80 min Scan# 455

Delta R.T. 0.00 min

Lab File: VU039871.D




Acq: 14 Aug 2020 20:08


Tgt Ion: 76 Resp: 1404

Ion Ratio Lower Upper

76 100

78 13.7 7.8 11.6#


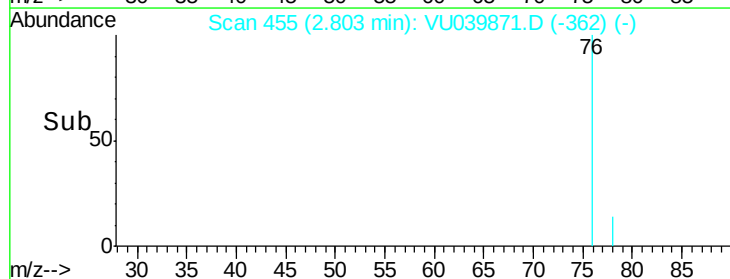
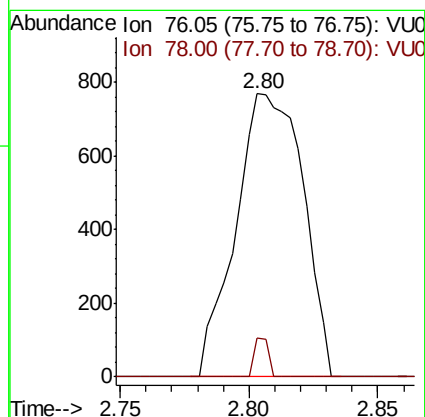
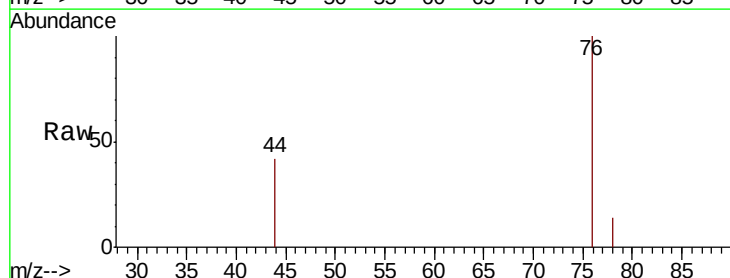


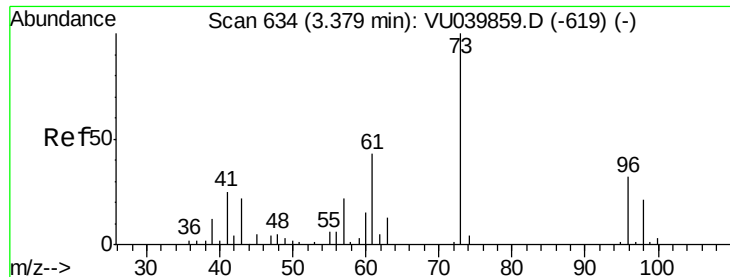

#17
Methyl tert-butyl Ether
Concen: 0.423 ug/L
RT: 3.39 min Scan# 636
Delta R.T. 0.01 min
Lab File: VU039871.D
Acq: 14 Aug 2020 20:08




Instrument :
MSVOA_U
ClientSampled :


Tot Ion: 73 Resp: 4624
Ion Ratio Lower Upper
73 100
43 29.4 18.2 27.4#
57 14.4 17.8 26.8#

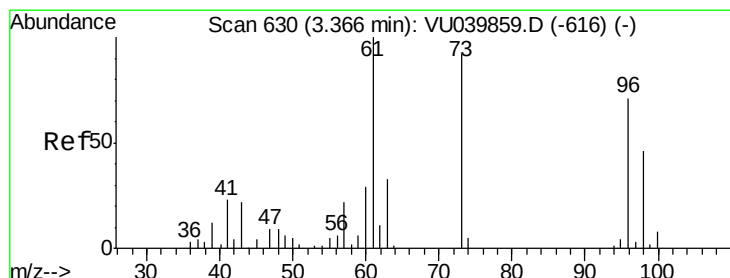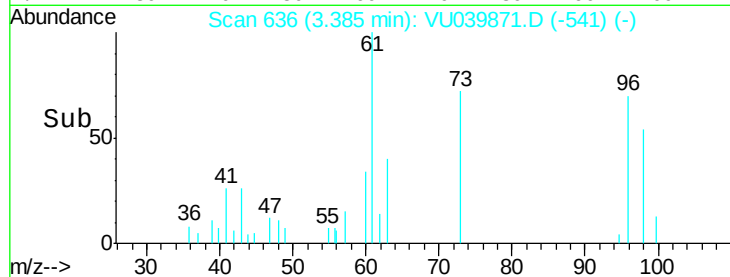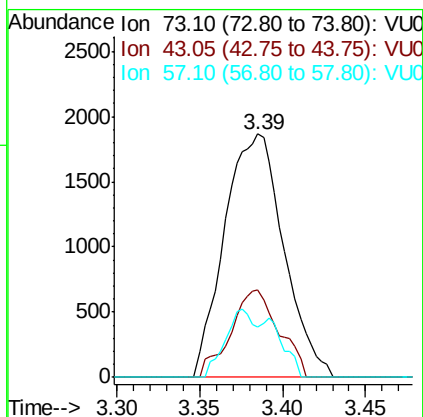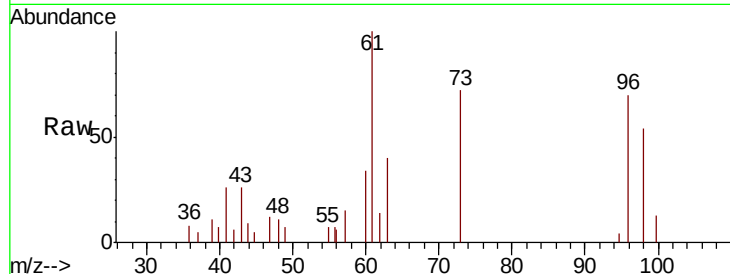

#18
trans-1,2-Dichloroethene
Concen: 1.577 ug/L
RT: 3.37 min Scan# 631
Delta R.T. 0.00 min
Lab File: VU039871.D
Acq: 14 Aug 2020 20:08

Tgt Ion: 96 Resp: 7230
Ion Ratio Lower Upper
96 100
61 156.5 96.5 179.1
98 73.4 40.9 76.0

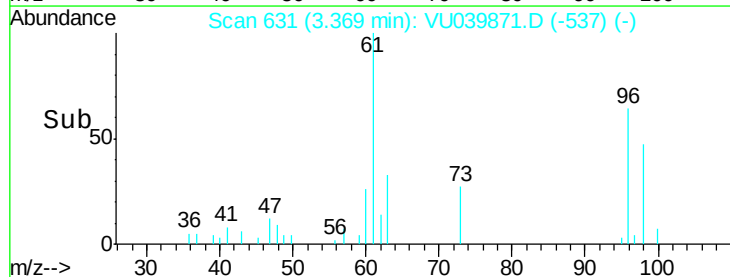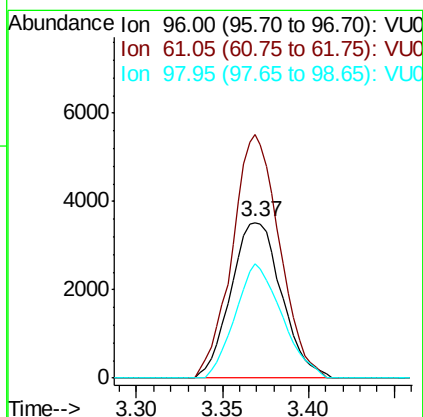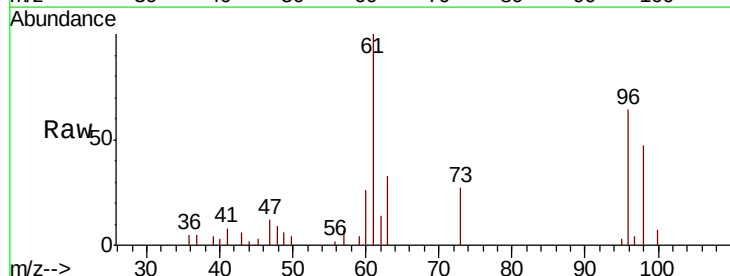

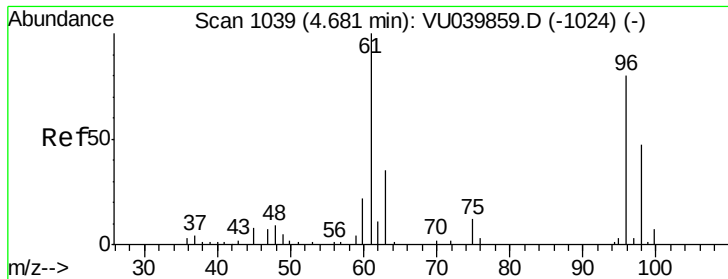

#22

cis-1,2-Dichloroethene

Concen: 0.437 ug/L

RT: 4.69 min Scan# 1043

Delta R.T. 0.01 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08

Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 96 Resp: 2178

Ion Ratio Lower Upper




96 100

61 159.5 87.4 162.2

68 0.0 0.0 0.0

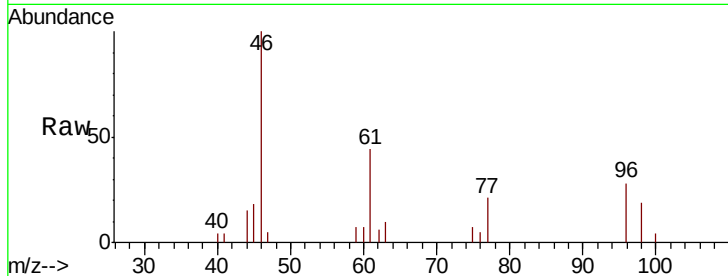

Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 68.15 (67.85 to 68.85): VU0

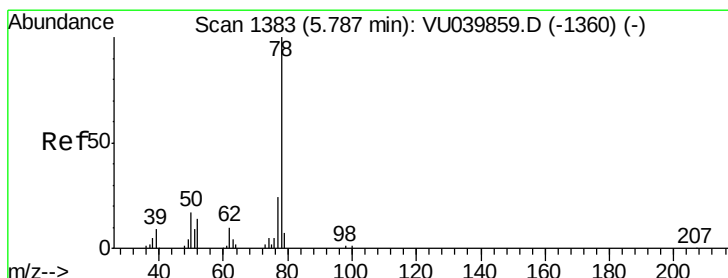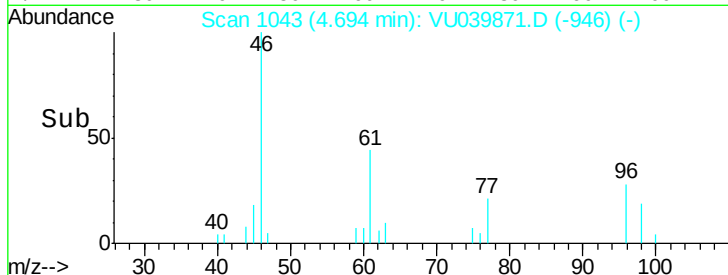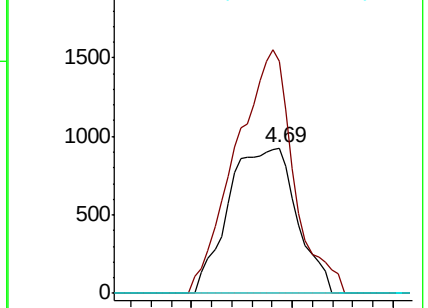

#33

Benzene

Concen: 0.159 ug/L


RT: 5.79 min Scan# 1383

Delta R.T. 0.00 min



Lab File: VU039871.D


Acq: 14 Aug 2020 20:08

Tgt Ion: 78 Resp: 3061

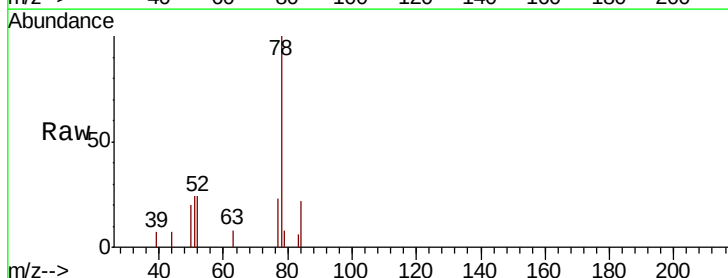

Abundance Ion 78.10 (77.80 to 78.80): VU0

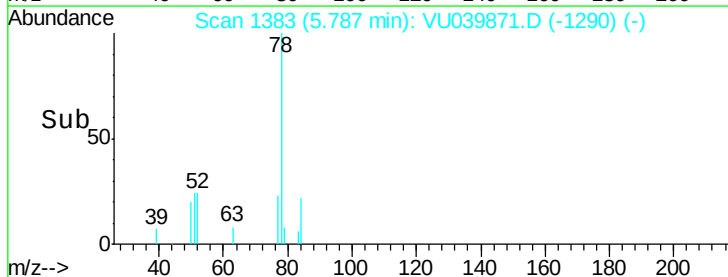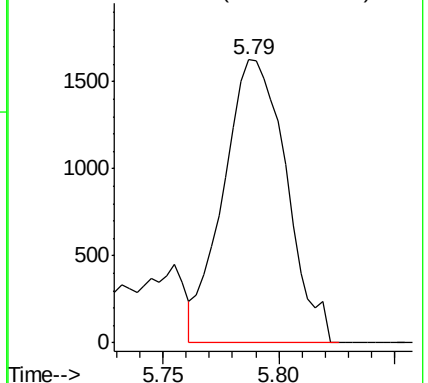

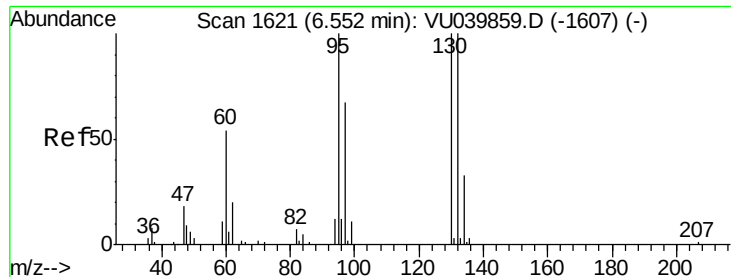

#34

Trichloroethene

Concen: 0.257 ug/L

RT: 6.55 min Scan# 1621

Delta R.T. 0.00 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08

Instrument :

MSVOA_U

ClientSampled :

Tot Ion: 95 Resp: 1287


Ion Ratio Lower Upper

95 100

97 52.9 44.0 81.8

132 82.9 71.7 133.3

130 95.2 71.1 132.1



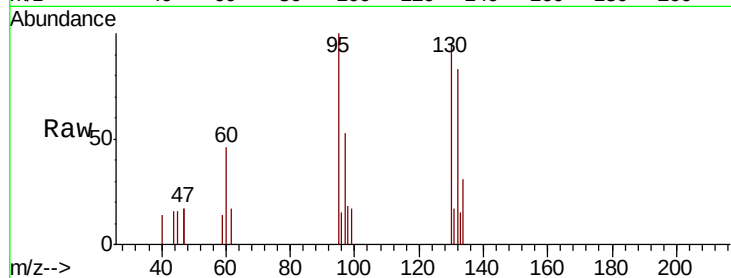


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

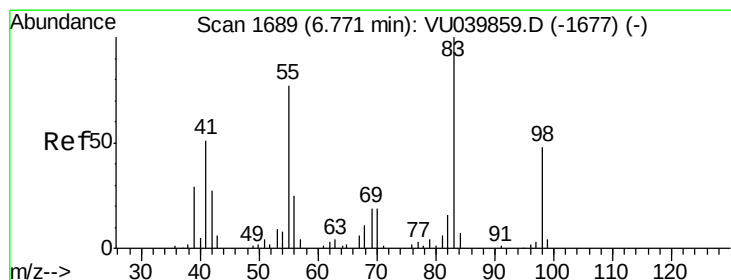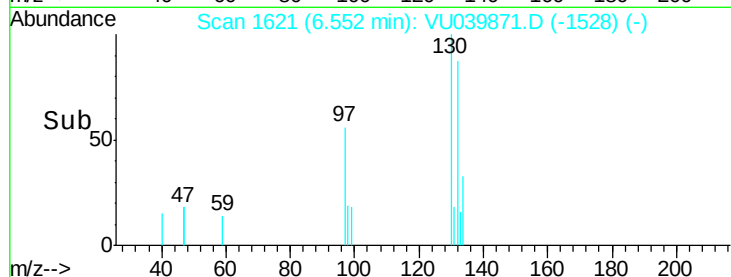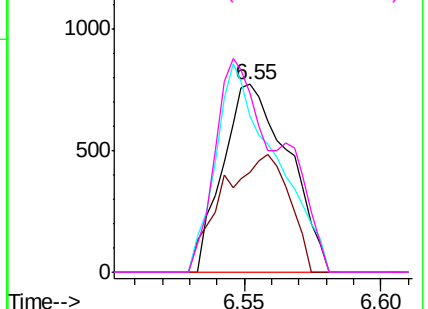

#35

Methylcyclohexane

Concen: 0.837 ug/L

RT: 6.70 min Scan# 1667

Delta R.T. -0.07 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08


Tgt Ion: 83 Resp: 6684

Ion Ratio Lower Upper

83 100

55 0.0 59.4 89.0#



98 0.8 39.0 58.4#

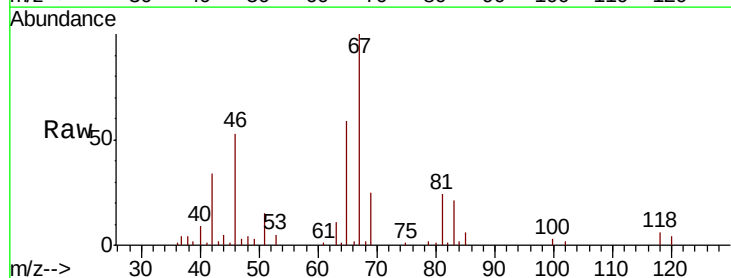


Abundance Ion 83.15 (82.85 to 83.85): VU0

Ion 55.10 (54.80 to 55.80): VU0

Ion 98.15 (97.85 to 98.85): VU0



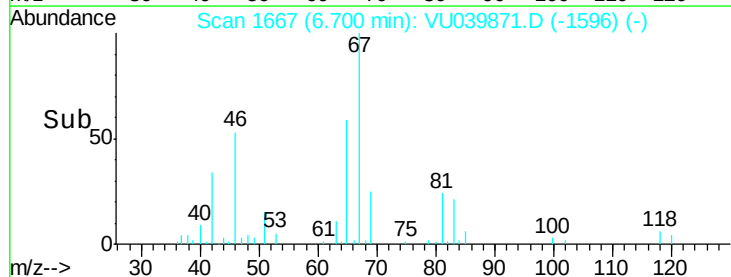
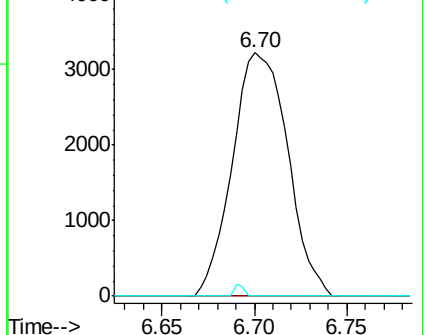


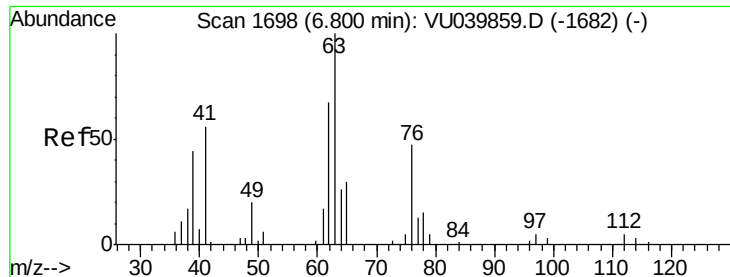

#37
 1,2-Dichloropropane
 Concen: 0.619 ug/L
 RT: 6.70 min Scan# 1667
 Delta R.T. -0.10 min
 Lab File: VU039871.D
 Acq: 14 Aug 2020 20:08




Instrument :
 MSVOA_U
 ClientSampled :


Tot Ion: 63 Resp: 3167
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.6#

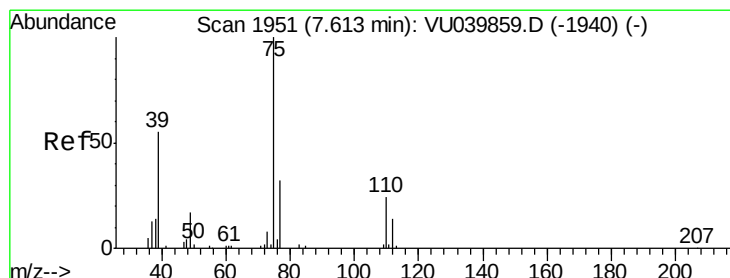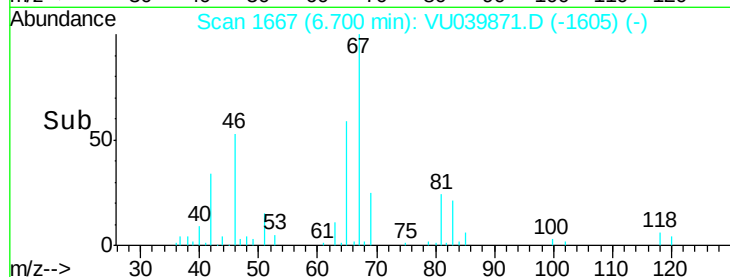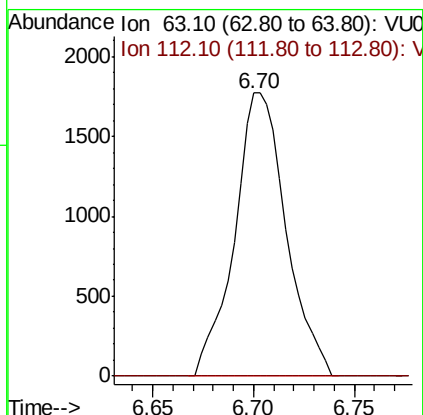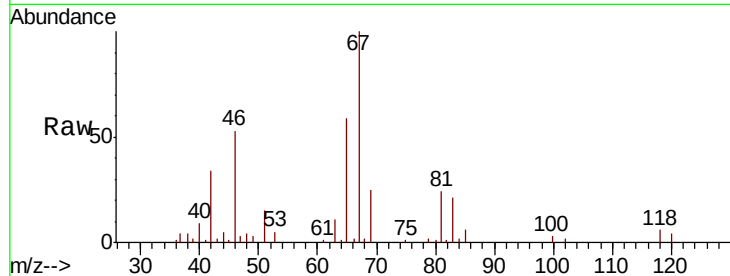

#39
 cis-1,3-Dichloropropene
 Concen: 0.112 ug/L
 RT: 7.57 min Scan# 1939
 Delta R.T. -0.04 min
 Lab File: VU039871.D
 Acq: 14 Aug 2020 20:08

Tgt Ion: 75 Resp: 779
 Ion Ratio Lower Upper
 75 100
 77 52.9 22.4 41.6#

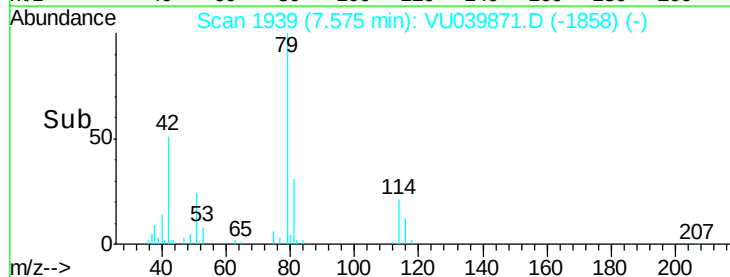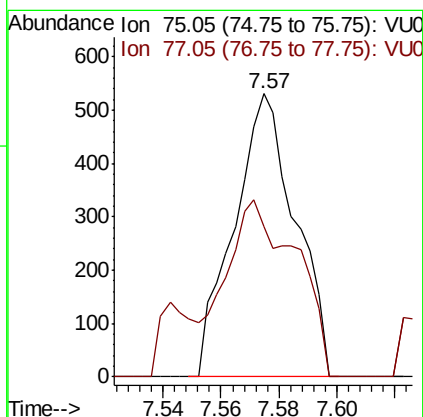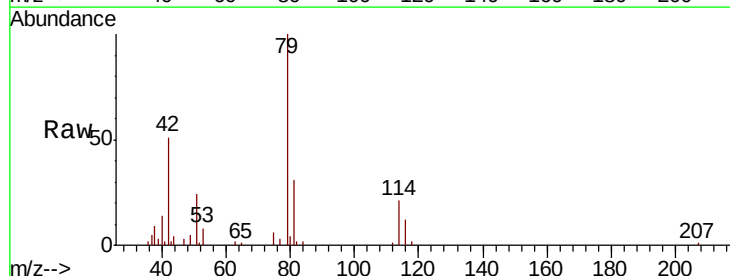

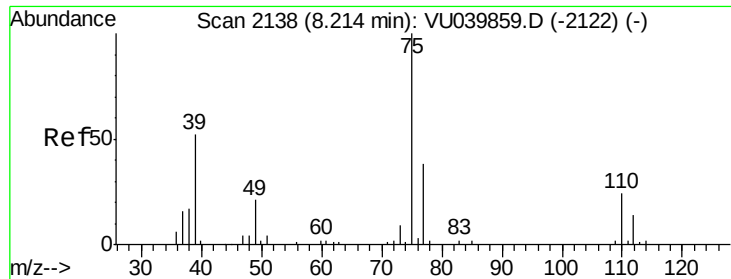

#44

trans-1,3-Dichloropropene

Concen: 0.123 ug/L

RT: 8.18 min Scan# 2128

Delta R.T. -0.03 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08


Instrument :
MSVOA_U
ClientSampled :

Tot Ion: 75 Resp: 771




Ion Ratio Lower Upper

75 100

77 476.5 21.6 40.2#

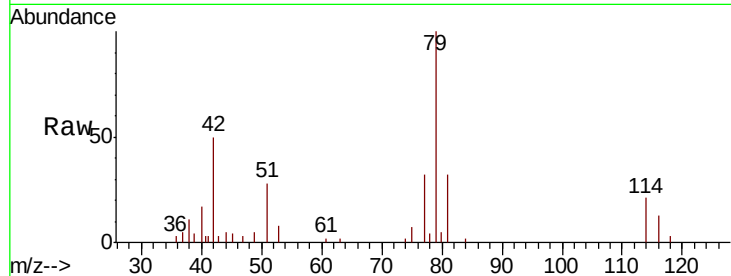

Abundance Ion 75.05 (74.75 to 75.75): VU0
Ion 77.05 (76.75 to 77.75): VU0

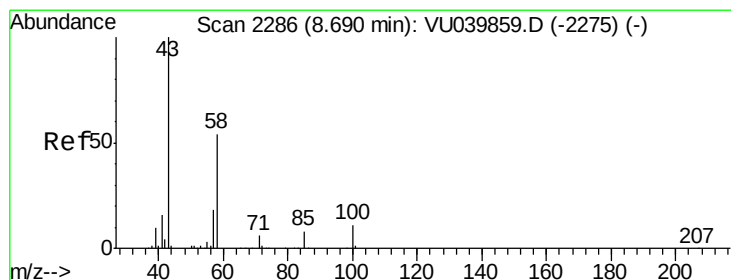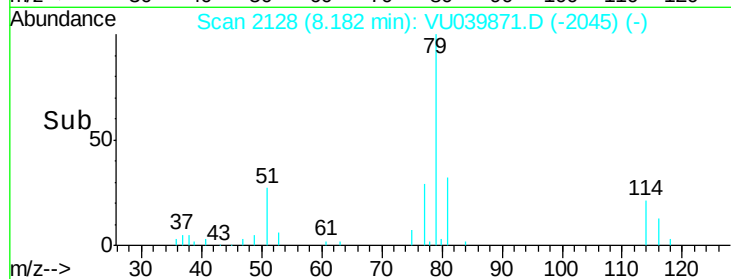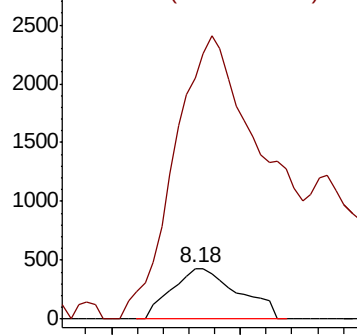

#48

2-Hexanone

Concen: 2.639 ug/L

RT: 8.64 min Scan# 2270

Delta R.T. -0.05 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08

Tgt Ion: 43 Resp: 7290


Ion Ratio Lower Upper

43 100



58 25.2 41.8 62.8#


57 29.0 14.2 21.4#

100 0.0 9.4 14.2#

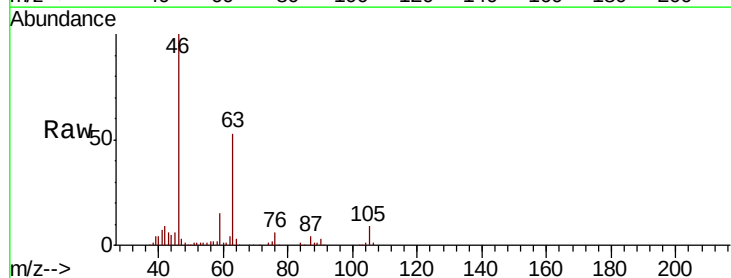

Abundance Ion 43.05 (42.75 to 43.75): VU0
Ion 58.05 (57.75 to 58.75): VU0
Ion 57.20 (56.90 to 57.90): VU0
Ion 100.15 (99.85 to 100.85): VU0

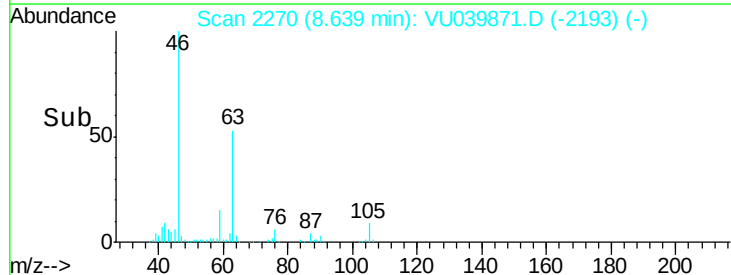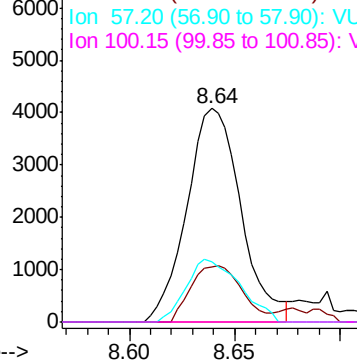

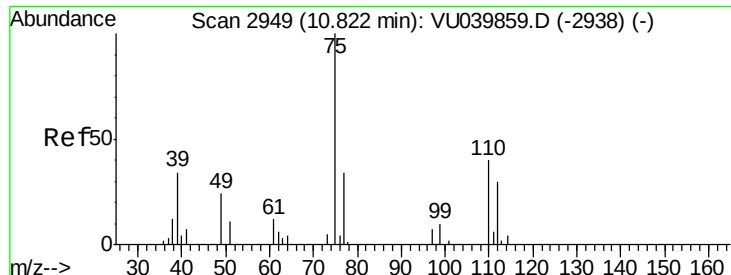

#59

1,2,3-Trichloropropane

Concen: 1.277 ug/L

RT: 11.81 min Scan# 3256

Delta R.T. 0.99 min

Lab File: VU039871.D

Acq: 14 Aug 2020 20:08

Instrument :

MSVOA_U

ClientSampleId :

Tot Ion: 75 Resp: 4715

Ion Ratio Lower Upper

75 100

77 38.1 24.6 37.0#

