


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081420\
Data File : VU039858.D
Acq On : 14 Aug 2020 13:15
Operator : SY/MD
Sample : BFB14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB14

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 18 07:51:41 2020

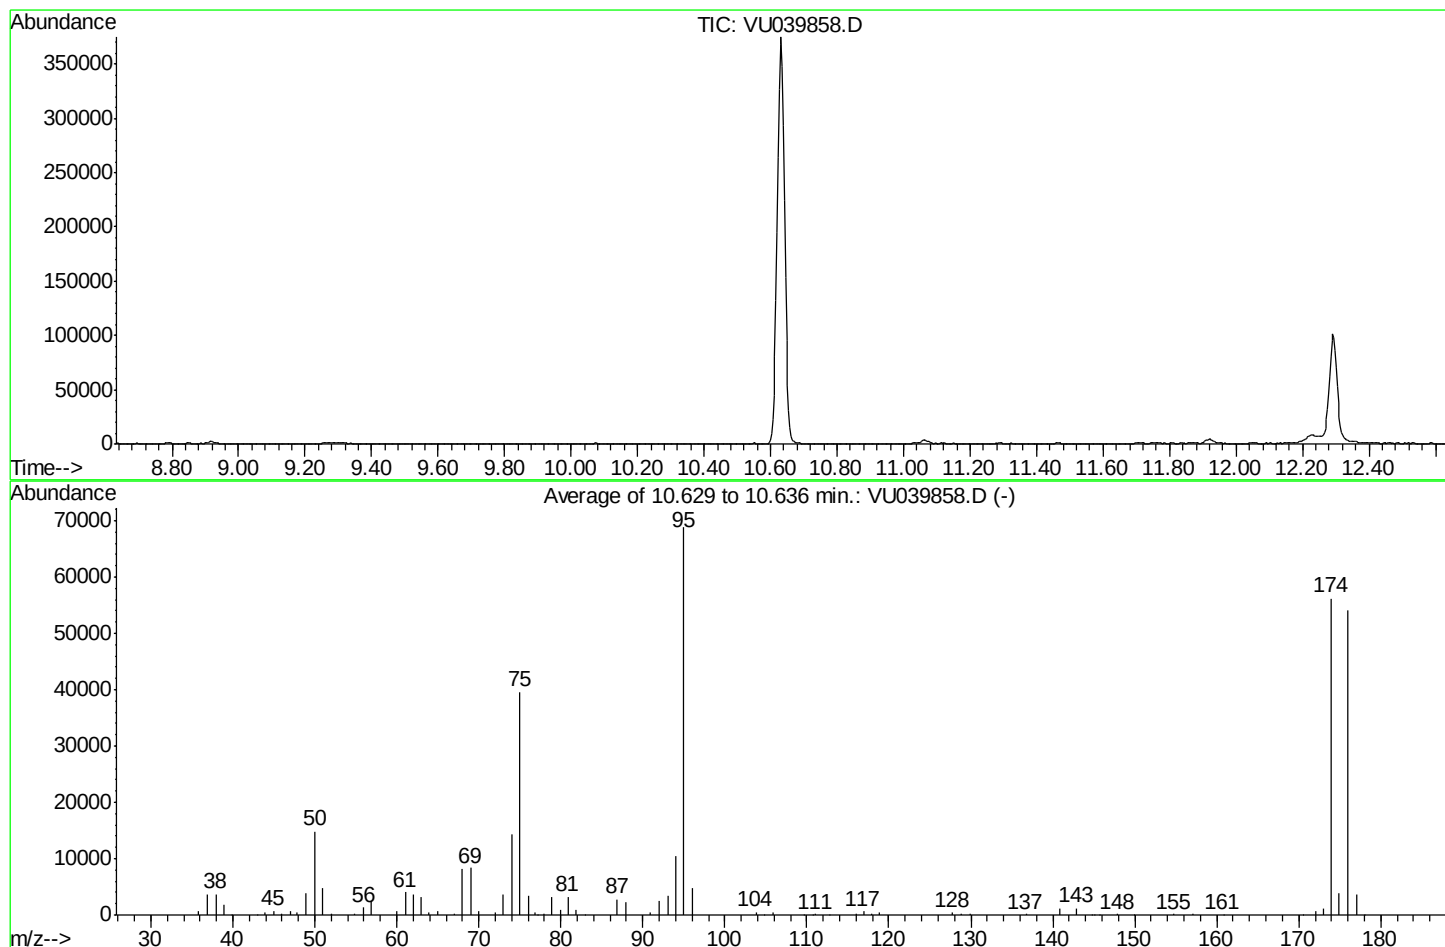

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	14828	PASS
75	95	30	80	57.5	39568	PASS
95	95	100	100	100.0	68845	PASS
96	95	5	9	7.1	4868	PASS
173	174	0.00	2	1.8	1039	PASS
174	95	50	120	81.7	56256	PASS
175	174	5	9	7.0	3924	PASS
176	174	95	101	96.1	54037	PASS
177	176	5	9	6.6	3558	PASS

m/z	Abundance
43.90	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
35.80	755.0
3 .90	3719.0
37.90	3888.0
38.90	1993.0
39.80	141.0
43.00	117.0
43.90	807.0
44.90	8 9.0
45.80	1 .0
47.00	754.0
47.80	3 0.0
48.90	3933.0
50.00	1509 .0
51.00	5133.0
52.10	125.0
54.90	224.0
5 .00	1350.0
5 .90	2409.0
0.00	829.0
1.00	4082.0
2.00	3875.0
3.00	3200.0
3.90	458.0
5.10	788.0
7.00	229.0
7.90	8 75.0
9.00	871 .0
70.10	80.0
71.90	3 1.0
72.90	3 .0
74.00	1457 .0
75.00	40552.0
7 .00	3523.0
7 .90	359.0
77.20	3 9.0
77.90	199.0
78.90	3338.0
79.90	1192.0
80.90	3489.0
81.90	959.0
82.90	11 .0
8 .90	30 7.0
87.90	2275.0
90.90	384.0
91.90	257 .0
93.00	3522.0
94.00	1037 .0
95.00	9800.0
9 .00	5100.0
103.80	53 .0
105.90	378.0
110.70	101.0
111.10	138.0
115.90	341.0
11 .90	17.0
117.90	339.0
118.90	29.0
127.80	3 0.0
128.80	1 2.0
129.90	2 9.0
13 .80	131.0
140.90	1014.0
142.90	118 .0
145.10	132.0
145.80	104.0
147.90	174.0
149.90	123.0
154.80	210.0
157.00	158.0
1 0.90	118.0
170. 0	104.0
172.10	793.0
173.00	985.0
174.00	55824.0
175.00	370 .0
17 .00	53328.0
177.00	3414.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
35.80	58.0
3 .90	3739.0
37.90	3871.0
38.90	1809.0
43.90	787.0
44.90	7 9.0
45.90	14 .0
47.10	755.0
47.80	399.0
48.90	3941.0
50.00	15290.0
51.00	5005.0
52.00	159.0
54.80	159.0
5 .00	12 1.0
5 .90	2 43.0
0.00	792.0
1.00	41 5.0
2.00	3809.0
3.00	3278.0
3.90	405.0
5.10	738.0
7.10	194.0
7.90	8520.0
9.00	8 55.0
70.00	707.0
72.00	423.0
72.90	3729.0
74.00	14829.0
75.00	40912.0
7 .00	3494.0
7 .90	459.0
78.00	209.0
78.90	33 2.0
79.90	1017.0
80.90	3375.0
81.90	1001.0
83.00	12 .0
8 .90	2851.0
88.00	2421.0
90.80	414.0
91.90	2 1.0
93.00	34 0.0
94.00	10777.0
95.00	71072.0
9 .00	5059.0
103.80	571.0
105.90	418.0
109.70	121.0
111.10	140.0
112.80	100.0
115.90	321.0
11 .90	8.0
117.90	282.0
118.90	590.0
127.80	37 .0
128.90	1 3.0
130.00	2 0.0
13 .70	192.0
140.90	115 .0
142.90	1272.0
145.00	110.0
147.90	155.0
154.80	199.0
157.00	159.0
1 0.80	122.0
172.10	777.0
173.00	1108.0
174.00	58128.0
174.90	39 .0
17 .00	5577 .0
177.00	3 38.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
35.80	537.0
3 .90	3533.0
37.90	3510.0
38.90	1554.0
43.90	791.0
45.00	08.0
4 .00	12 .0
47.10	718.0
47.90	393.0
49.00	3432.0
50.00	14100.0
50.90	4399.0
52.00	17 .0
54.70	159.0
5 .00	1211.0
5 .90	2585.0
0.00	701.0
1.00	372.0
2.00	352 .0
3.00	3173.0
3.90	324.0
5.00	593.0
7.00	171.0
7.90	7433.0
9.00	7839.0
70.00	715.0
72.00	420.0
73.00	3525.0
74.00	1380 .0
75.00	37240.0
7 .00	298.0
7 .90	487.0
78.00	249.0
78.90	3111.0
79.90	808.0
80.90	3034.0
81.90	948.0
83.00	122.0
8 .90	2409.0
88.00	2344.0
90.80	408.0
92.00	2391.0
93.10	30 .0
94.00	9994.0
95.00	54.0
9 .00	4445.0
103.80	474.0
104.80	105.0
105.80	437.0
111.00	148.0
112.70	112.0
11 .00	284.0
11 .90	97.0
117.80	20.0
118.90	450.0
127.80	327.0
128.90	13.0
129.90	20.0
13 .70	211.0
140.90	1033.0
142.90	1238.0
144.80	13 .0
145.70	100.0
147.90	13 .0
154.80	152.0
157.10	117.0
10.70	11 .0
170.40	107.0
172.00	77.0
173.00	102 .0
174.00	5481 .0
174.90	4100.0
17 .00	53008.0
177.00	322.0
178.00	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14