

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081424\
 Data File : VU060446.D
 Acq On : 14 Aug 2024 12:16
 Operator : MD/SY
 Sample : VIBLK126
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK126

Quant Time: Aug 14 17:16:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 14 01:18:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	89996	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	91308	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	38145	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	33250	4.707	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	94.200%	
7) Chloroethane-d5	1.907	69	30272	4.752	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.000%	
11) 1,1-Dichloroethene-d2	2.554	65	15111	5.026	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	100.600%	
20) 2-Butanone-d5	4.640	46	68434	45.647	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	91.300%	
24) Chloroform-d	5.055	84	68155	4.872	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	5.695	65	34582	5.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.600%	
32) Benzene-d6	5.721	84	134246	4.875	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
36) 1,2-Dichloropropane-d6	6.685	67	42916	5.024	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.400%	
41) Toluene-d8	7.894	98	110844	4.509	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.200%	
43) trans-1,3-Dichloroprop...	8.177	79	13740	4.976	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.600%	
46) 2-Hexanone-d5	8.640	63	54851	44.760	ug/L	0.01
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.520%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	33199	4.737	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152	37727	5.369	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.400%	
Target Compounds						
16) Methylene chloride	3.036	84	1929	0.229	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081424\
Data File : VU060446.D
Acq On : 14 Aug 2024 12:16
Operator : MD/SY
Sample : VIBLK126
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK126

Quant Time: Aug 14 17:16:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 14 01:18:59 2024
Response via : Initial Calibration

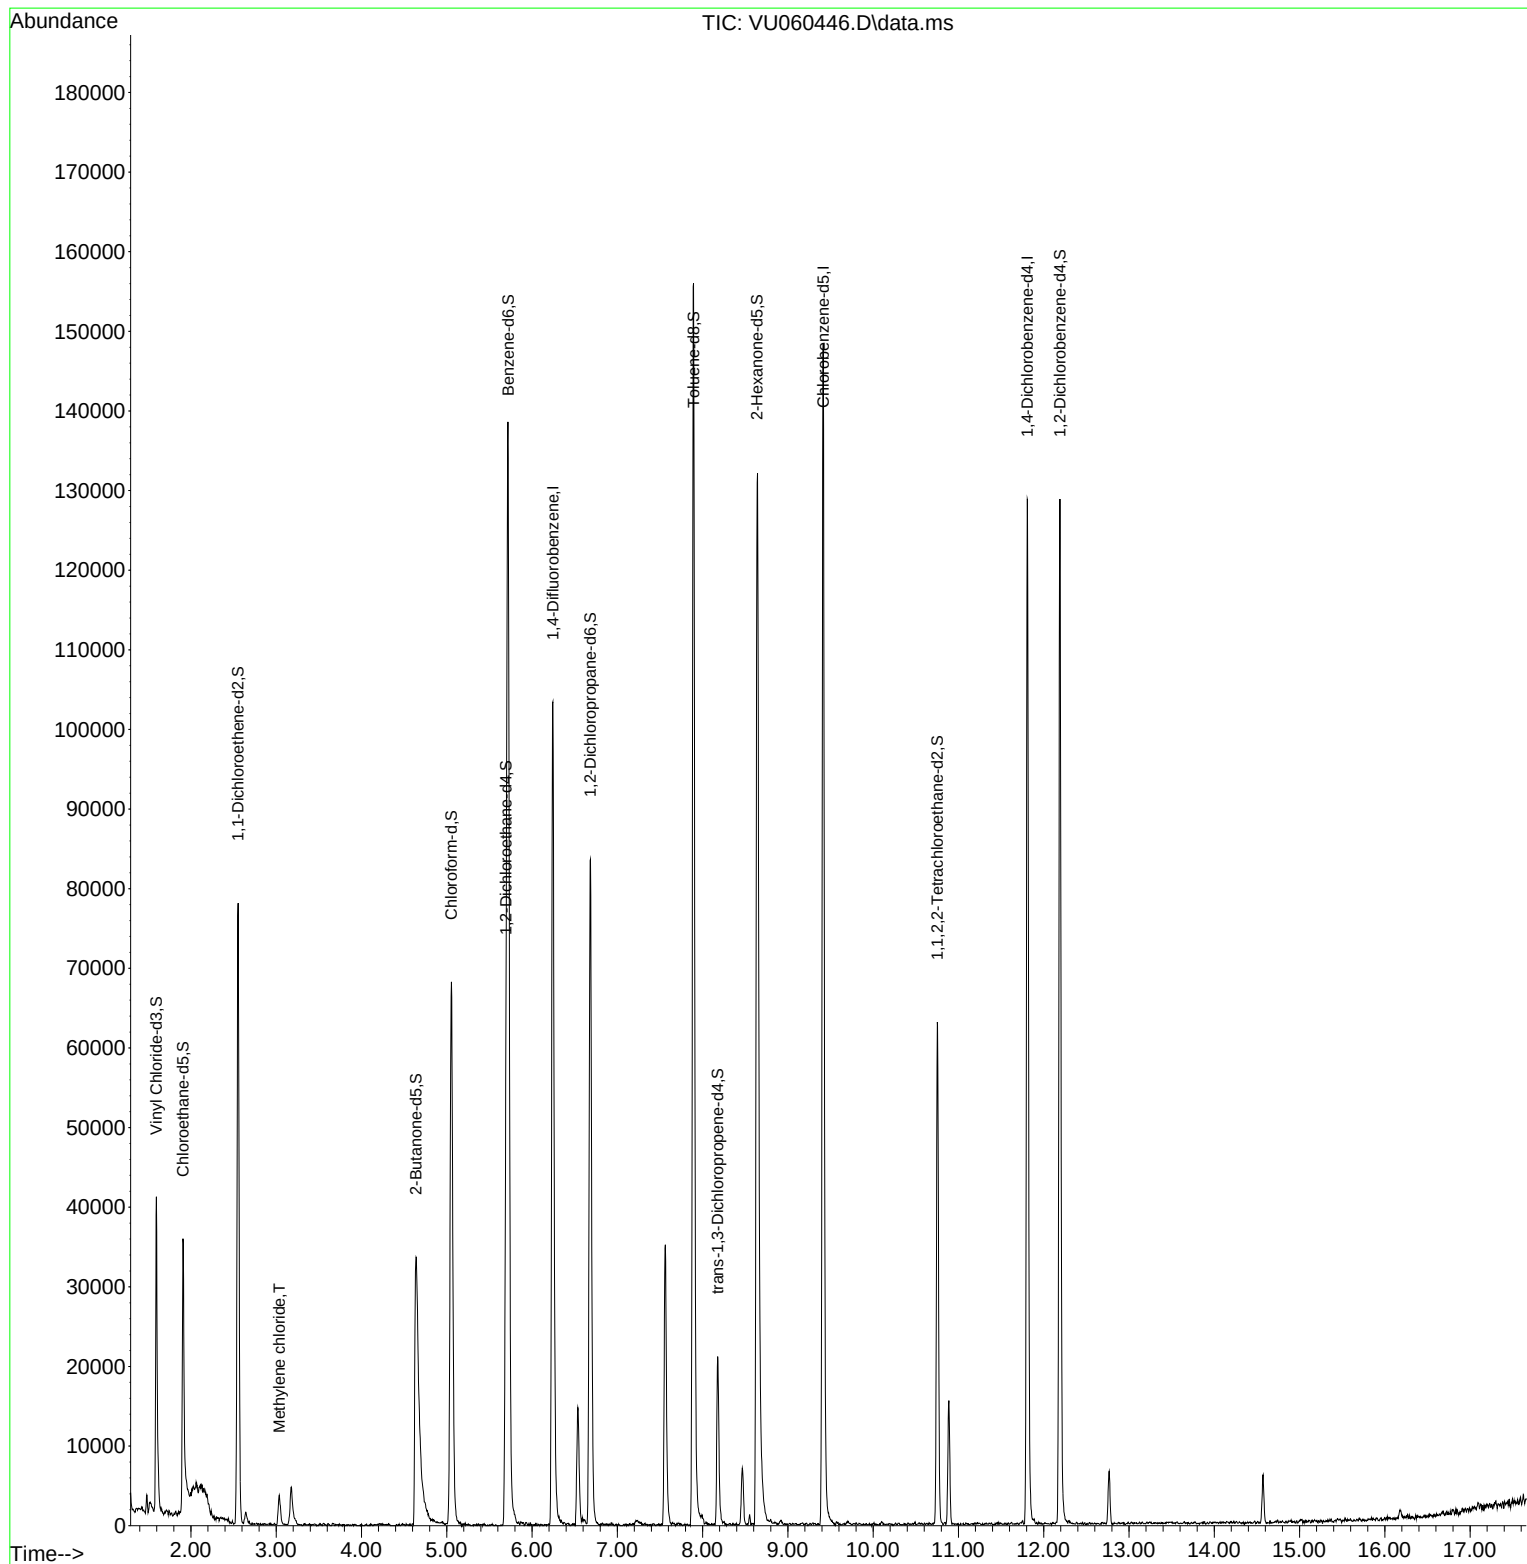

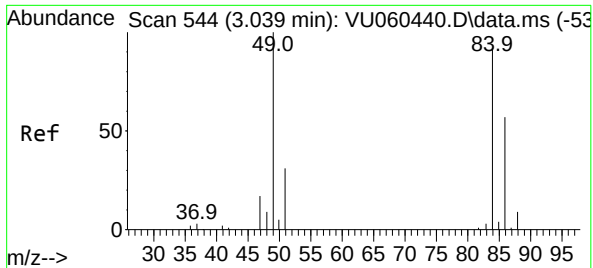

#16
Methylene chloride
Concen: 0.229 ug/L
RT: 3.036 min Scan# 54
Delta R.T. -0.003 min
Lab File: VU060446.D
Acq: 14 Aug 2024 12:16

Instrument :
MSVOA_U
ClientSampleId :
VIBLK126

Tgt Ion:	84	Resp:	1929
Ion	Ratio	Lower	Upper
84	100		
86	56.0	47.1	87.5
49	104.3	73.9	137.3

