


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081424\
Data File : VU060439.D
Acq On : 14 Aug 2024 08:33
Operator : MD/SY
Sample : BFB185
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB185

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Aug 14 01:18:59 2024

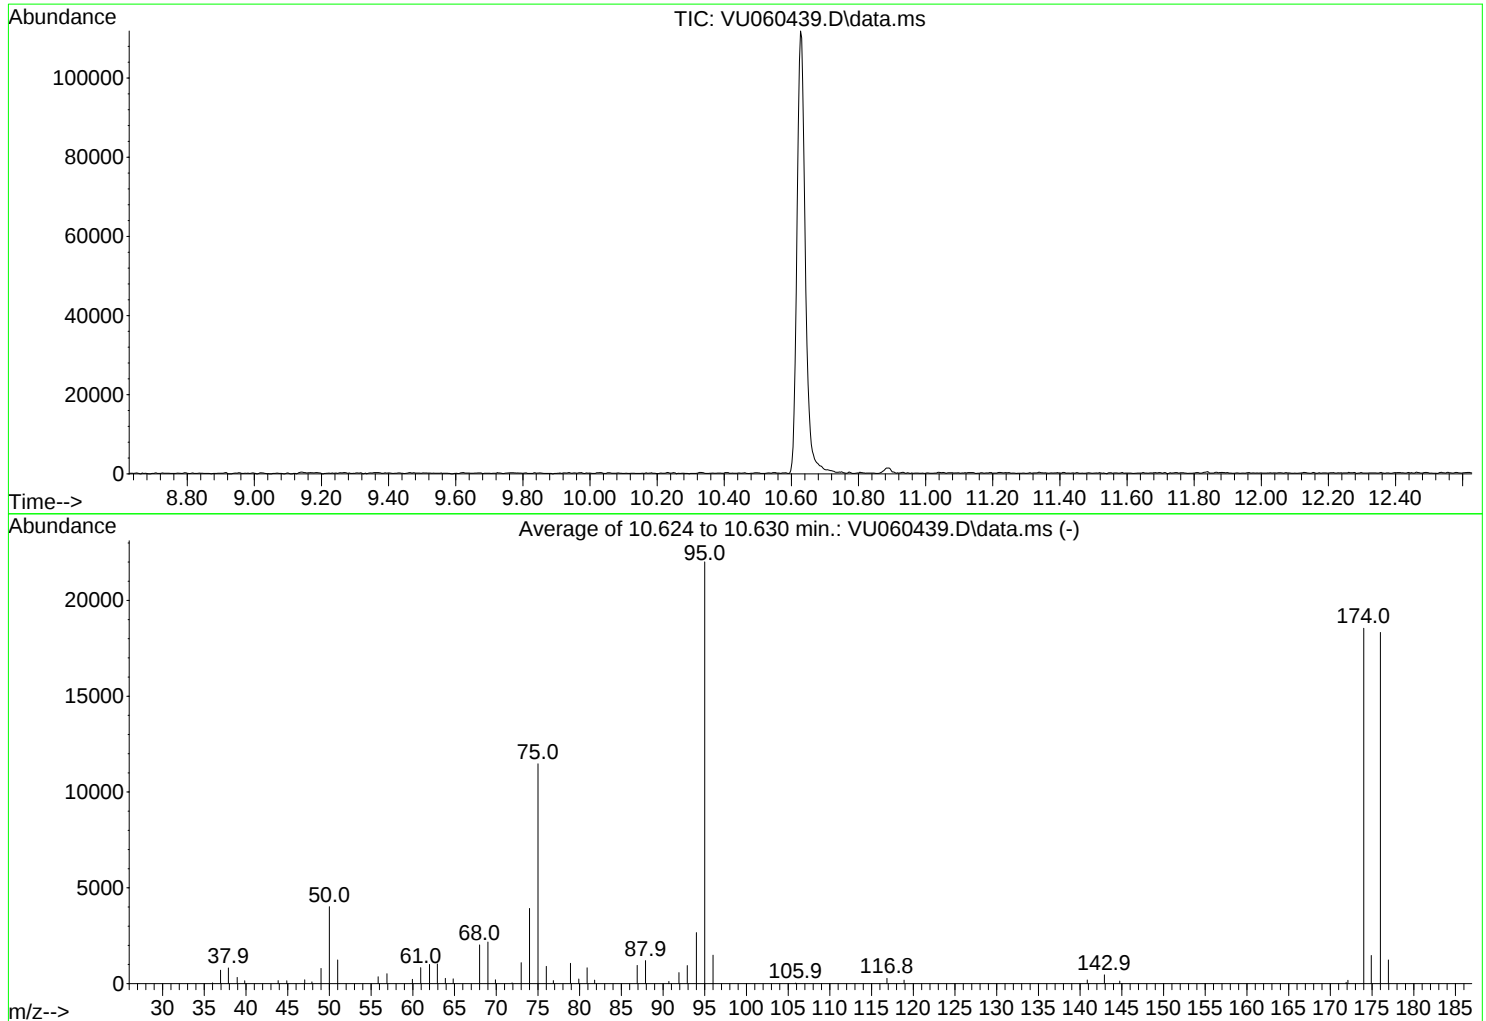

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	4019	PASS
75	95	30	80	52.1	11471	PASS
95	95	100	100	100.0	22013	PASS
96	95	5	9	6.8	1487	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.3	18549	PASS
175	174	5	9	7.9	1472	PASS
176	174	95	101	98.8	18333	PASS
177	176	5	9	6.8	1240	PASS

m/z	Abundance
43.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
36.90	642.0
37.90	735.0
38.90	292.0
39.90	133.0
43.90	265.0
44.90	126.0
47.00	220.0
47.90	159.0
49.00	881.0
50.00	4055.0
51.00	1206.0
55.80	391.0
56.90	526.0
60.00	196.0
60.90	938.0
62.00	928.0
62.90	982.0
63.90	248.0
64.80	215.0
68.00	1957.0
69.00	2114.0
69.90	197.0
73.00	1037.0
74.00	4002.0
75.00	10951.0
76.00	842.0
76.80	156.0
78.90	955.0
79.90	272.0
80.90	814.0
81.80	175.0
86.90	974.0
87.90	1179.0
90.70	110.0
91.90	547.0
92.90	917.0
94.00	2610.0
95.00	21072.0
96.00	1423.0
116.90	269.0
118.90	225.0
140.80	183.0
142.90	449.0
144.70	102.0
171.90	211.0
174.00	17448.0
174.90	1484.0
176.00	17112.0
176.90	1189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
37.00	705.0
37.90	828.0
39.00	332.0
39.90	164.0
43.90	285.0
44.90	163.0
47.10	206.0
47.90	129.0
49.00	829.0
50.00	4175.0
51.00	1278.0
55.80	357.0
56.90	526.0
59.90	235.0
60.90	840.0
62.00	1016.0
62.90	1008.0
63.90	289.0
64.90	265.0
68.00	2088.0
69.00	2219.0
69.90	205.0
73.00	1156.0
74.00	4024.0
75.00	11823.0
76.00	912.0
76.90	154.0
78.90	1126.0
79.90	248.0
80.90	825.0
81.80	184.0
86.90	982.0
87.90	1268.0
90.70	128.0
91.90	584.0
92.90	984.0
94.00	2745.0
95.00	22752.0
96.00	1503.0
116.80	313.0
118.90	181.0
140.90	191.0
142.90	477.0
144.70	128.0
172.10	231.0
174.00	19080.0
174.90	1540.0
176.00	18912.0
177.00	1262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
36.00	125.0
37.00	759.0
37.90	894.0
39.00	350.0
39.80	149.0
43.90	315.0
44.90	154.0
47.10	185.0
49.00	667.0
50.00	3827.0
51.00	1211.0
55.90	322.0
56.90	507.0
60.00	246.0
61.00	727.0
62.00	1063.0
63.00	1081.0
63.90	302.0
64.90	277.0
68.00	2017.0
69.00	2177.0
69.90	197.0
71.90	128.0
73.00	1099.0
74.00	3751.0
75.00	11639.0
76.00	965.0
76.90	160.0
78.90	1101.0
79.90	203.0
80.90	845.0
81.80	182.0
86.90	902.0
87.90	1157.0
90.70	105.0
91.90	591.0
92.90	935.0
94.00	2638.0
95.00	22216.0
96.00	1534.0
105.90	106.0
116.80	257.0
118.90	137.0
140.90	204.0
142.90	462.0
144.80	164.0
172.10	307.0
174.00	19120.0
174.90	1392.0
176.00	18976.0
177.00	1269.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185