


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081518\
Data File : VU026129.D
Acq On : 15 Aug 2018 07:27
Operator : MD/SY
Sample : BFB47
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081518WMA.M
Title : VOC Analysis
Last Update : Thu Aug 16 16:15:16 2018

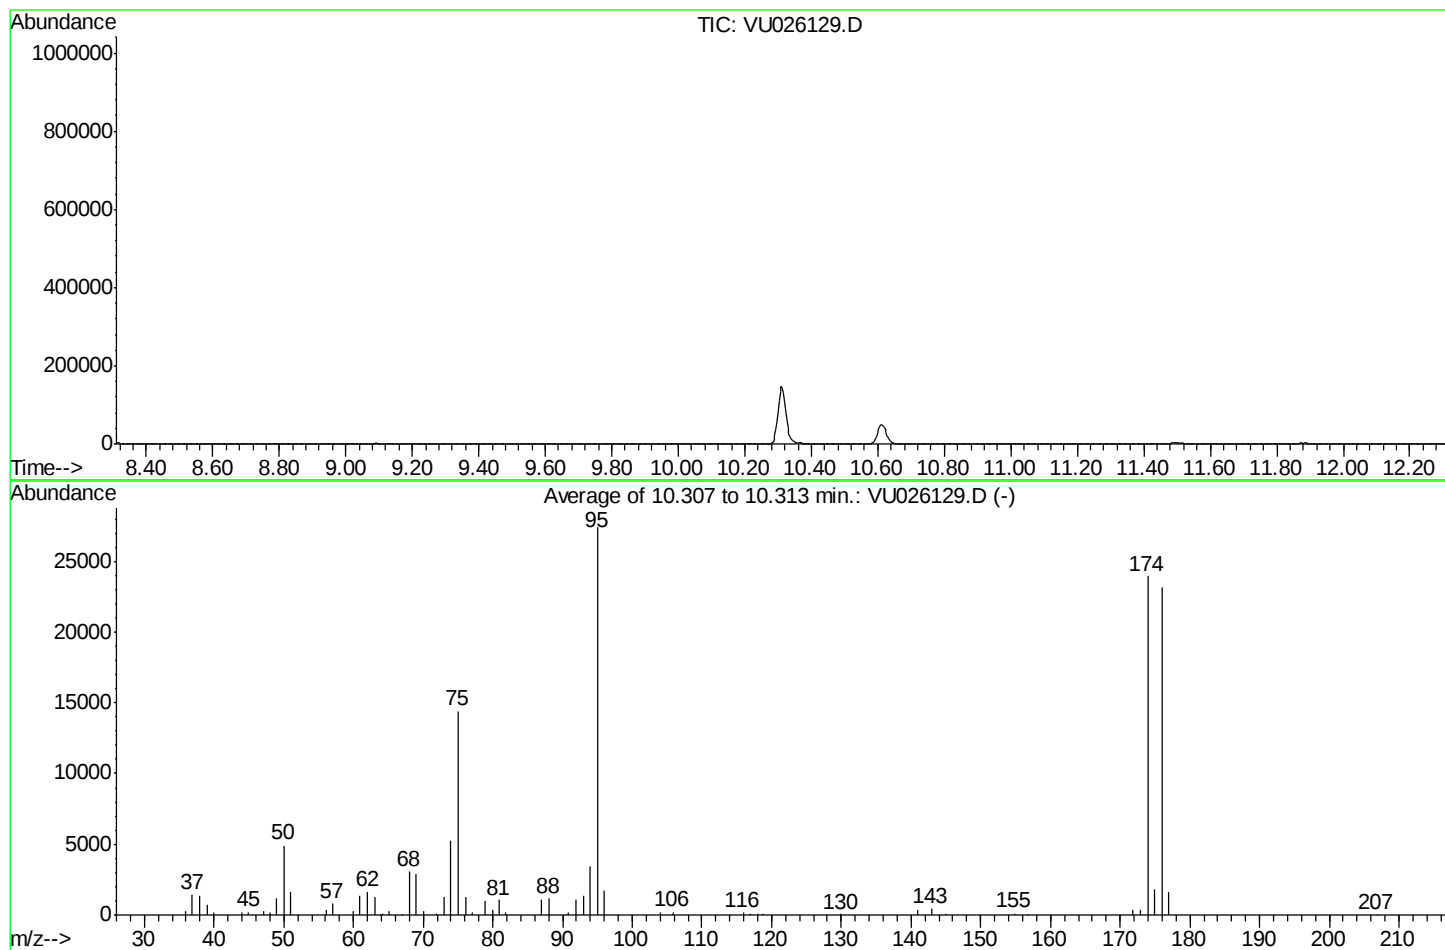

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	4922	PASS
75	95	30	80	52.6	14404	PASS
95	95	100	100	100.0	27397	PASS
96	95	5	9	6.1	1681	PASS
173	174	0.00	2	1.4	341	PASS
174	95	50	120	87.4	23946	PASS
175	174	5	9	7.6	1820	PASS
176	174	95	101	96.9	23192	PASS
177	176	5	9	7.0	1613	PASS

m/z	Abundance
44.00	347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	282.0
36.90	1331.0
38.00	1198.0
39.00	696.0
39.90	209.0
44.00	442.0
45.00	195.0
47.10	312.0
48.00	189.0
49.00	1177.0
50.00	4919.0
50.90	1686.0
56.10	345.0
57.00	764.0
59.90	251.0
60.90	1388.0
62.00	1497.0
63.00	1318.0
64.20	142.0
65.10	305.0
68.00	2926.0
69.00	2614.0
70.10	237.0
71.90	131.0
73.00	1259.0
74.00	5089.0
75.00	13938.0
76.00	1127.0
77.00	193.0
78.90	948.0
80.10	350.0
80.90	1015.0
81.90	184.0
87.00	1015.0
88.00	1046.0
90.80	186.0
92.00	996.0
93.00	1203.0
94.00	3464.0
95.00	26232.0
96.00	1617.0
104.00	164.0
105.90	145.0
115.90	172.0
116.80	124.0
118.00	106.0
118.70	130.0
140.90	427.0
142.90	410.0
144.90	125.0
154.90	103.0
171.80	341.0
173.00	288.0
174.00	22048.0
175.00	1663.0
176.00	21584.0
177.00	1564.0
206.80	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	309.0
36.90	1524.0
38.00	1395.0
39.00	710.0
39.90	167.0
44.00	531.0
45.00	218.0
47.10	292.0
48.10	212.0
49.00	1223.0
50.00	5154.0
51.00	1710.0
56.00	406.0
57.00	792.0
59.90	282.0
61.00	1481.0
62.00	1727.0
63.00	1360.0
64.20	132.0
65.10	329.0
68.00	3142.0
69.00	3028.0
70.10	258.0
71.90	106.0
73.00	1337.0
74.00	5449.0
75.00	14847.0
76.00	1339.0
77.00	218.0
78.90	998.0
80.00	368.0
80.90	1089.0
81.90	234.0
87.00	1171.0
88.00	1200.0
90.90	178.0
92.00	1137.0
93.00	1394.0
94.00	3604.0
95.00	28088.0
96.00	1750.0
104.00	152.0
105.80	187.0
115.90	182.0
116.80	132.0
118.00	127.0
118.70	138.0
130.00	106.0
140.90	408.0
142.90	460.0
145.00	107.0
154.90	110.0
171.90	373.0
172.90	358.0
174.00	24808.0
174.90	1858.0
176.00	23912.0
177.00	1675.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	328.0
36.90	1471.0
38.00	1386.0
39.00	656.0
40.00	127.0
44.10	563.0
45.00	236.0
47.00	256.0
48.10	211.0
49.00	1110.0
50.00	4695.0
51.00	1598.0
56.00	400.0
56.90	809.0
59.90	269.0
61.00	1317.0
62.00	1671.0
63.00	1263.0
63.90	138.0
65.10	305.0
66.90	105.0
68.00	3037.0
69.00	3114.0
70.00	231.0
73.00	1311.0
74.00	5291.0
75.00	14427.0
76.10	1446.0
77.10	240.0
78.90	983.0
80.00	304.0
80.90	1068.0
81.90	231.0
87.00	1091.0
88.00	1223.0
90.80	144.0
92.00	1068.0
93.00	1448.0
94.00	3364.0
95.00	27872.0
96.00	1678.0
103.90	110.0
105.80	219.0
115.90	140.0
116.90	126.0
117.90	176.0
118.80	135.0
130.00	111.0
140.90	385.0
142.90	469.0
154.80	114.0
156.80	110.0
171.90	421.0
172.90	377.0
174.00	24984.0
174.90	1941.0
176.00	24080.0
177.00	1600.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47