
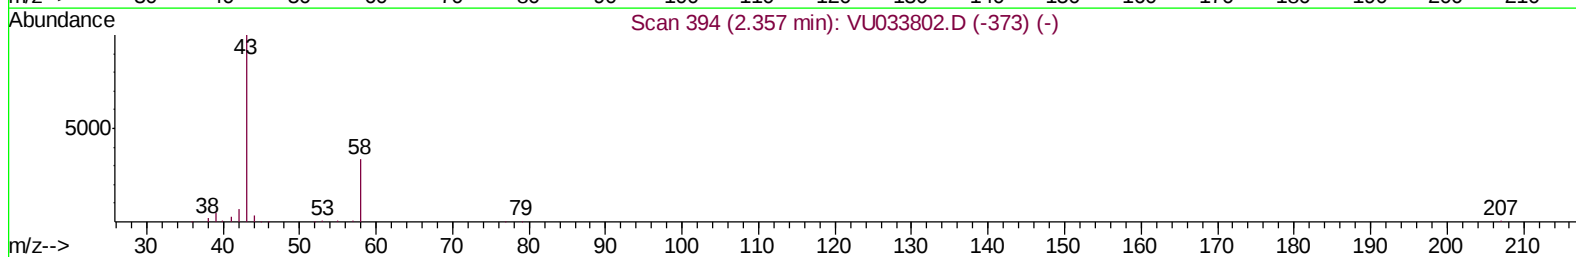
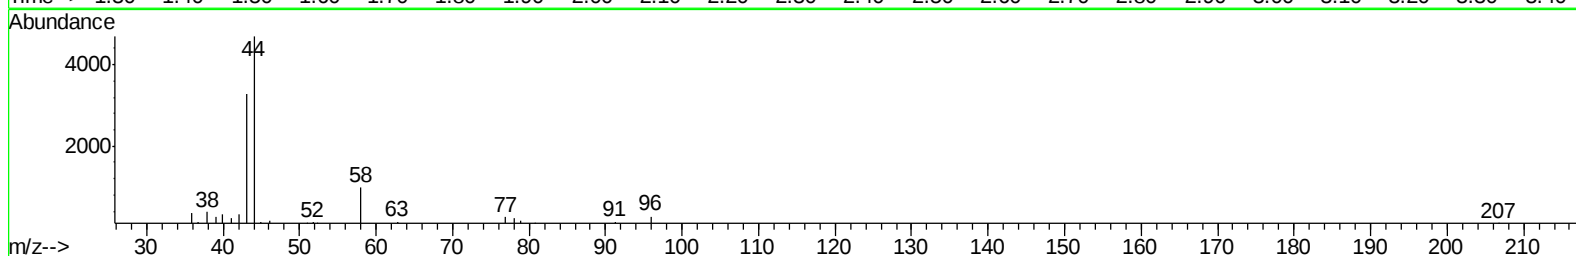


Data File : VU033804.D
Acq On : 15 Aug 2019 11:50
Operator : JC/SP
Sample : MDL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 16 01:11:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR081419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 01:09:16 2019
Response via : Initial Calibration

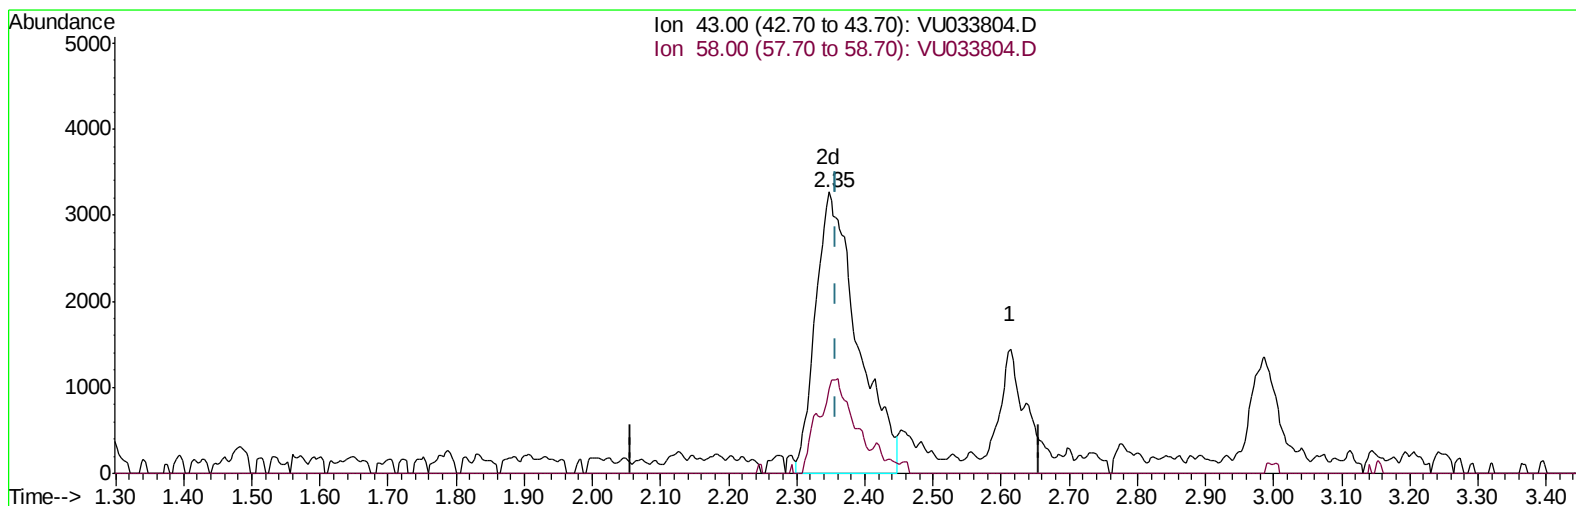

TIC: VU033804.D

(13) Acetone (T)

2.347min (-0.010) 3.21ug/L m

response 14003

Ion	Exp%	Act%
43.00	100	100
58.00	13.50	0.71
0.00	0.00	0.00
0.00	0.00	0.00