
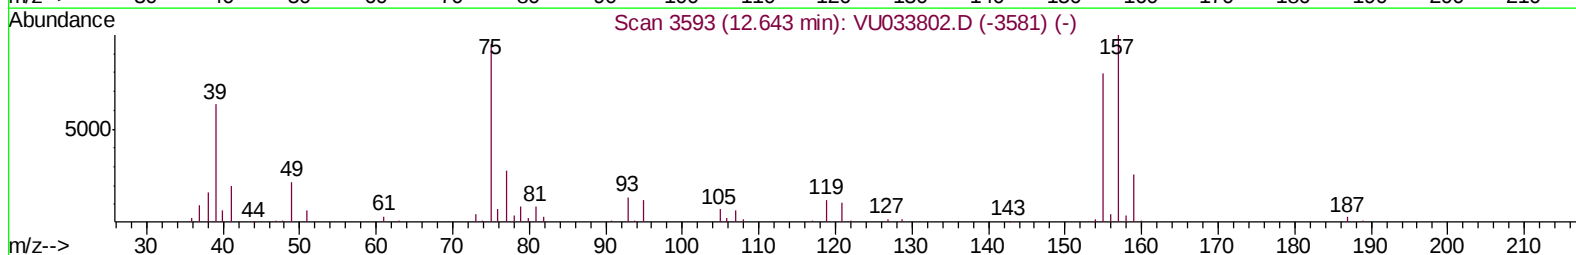
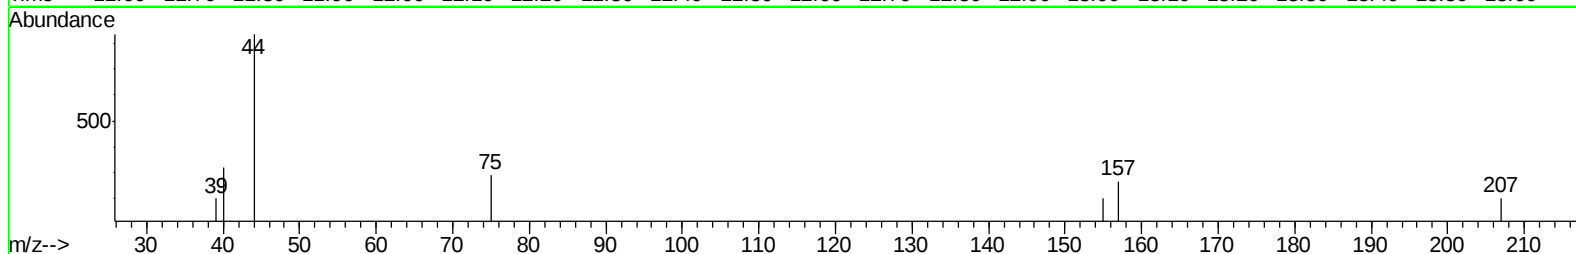


Data File : VU033805.D
Acq On : 15 Aug 2019 12:14
Operator : JC/SP
Sample : MDL04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 16 01:12:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR081419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 01:09:16 2019
Response via : Initial Calibration

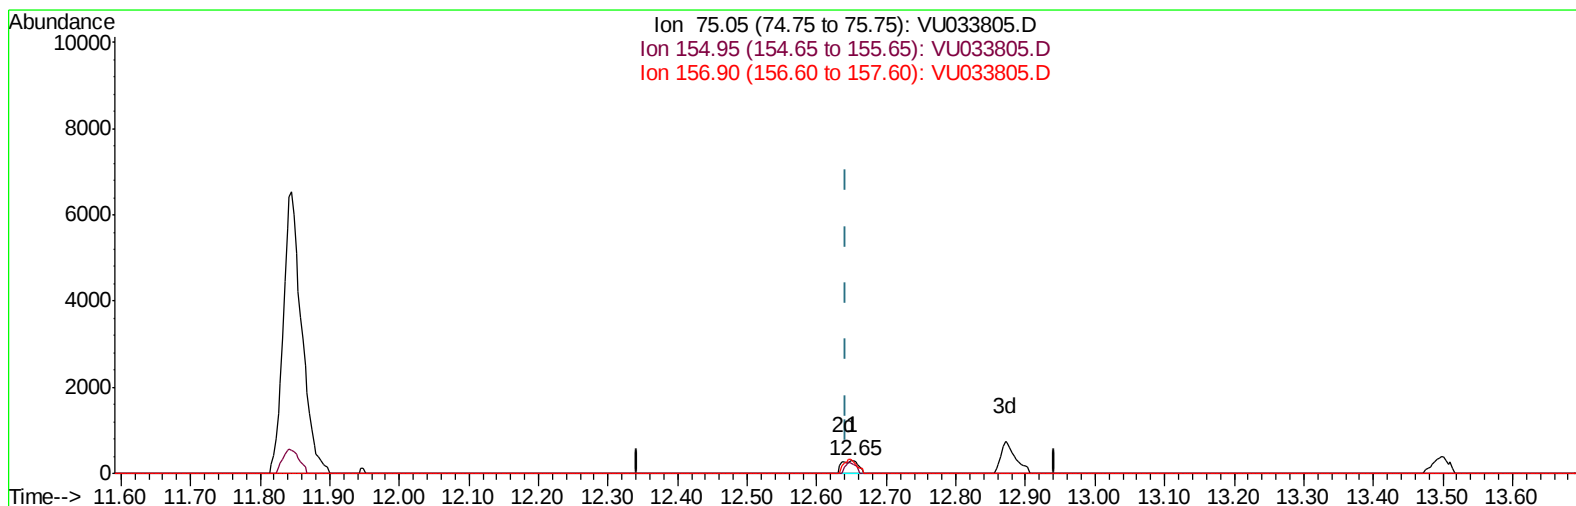

TIC: VU033805.D

(68) 1,2-Dibromo-3-chloropropane (T)

12.652min (+0.009) 0.21ug/L m

response 480

Ion	Exp%	Act%
75.05	100	100
154.95	84.10	69.07
156.90	106.60	91.41
0.00	0.00	0.00