
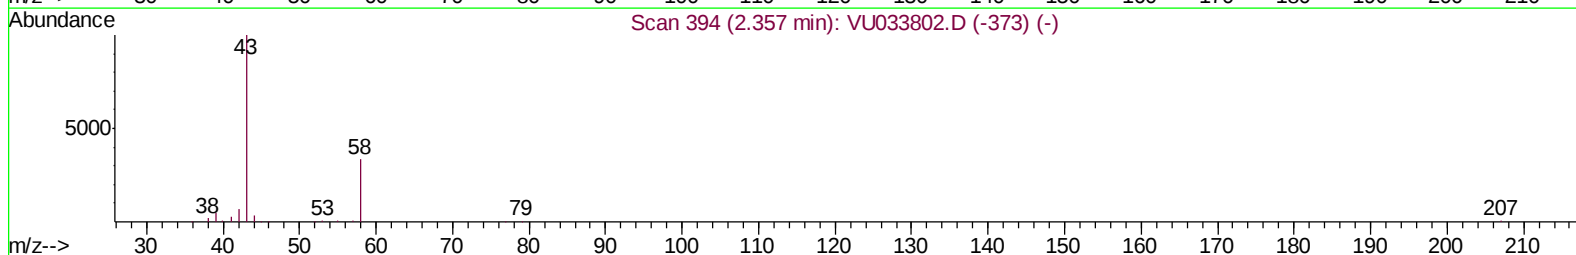
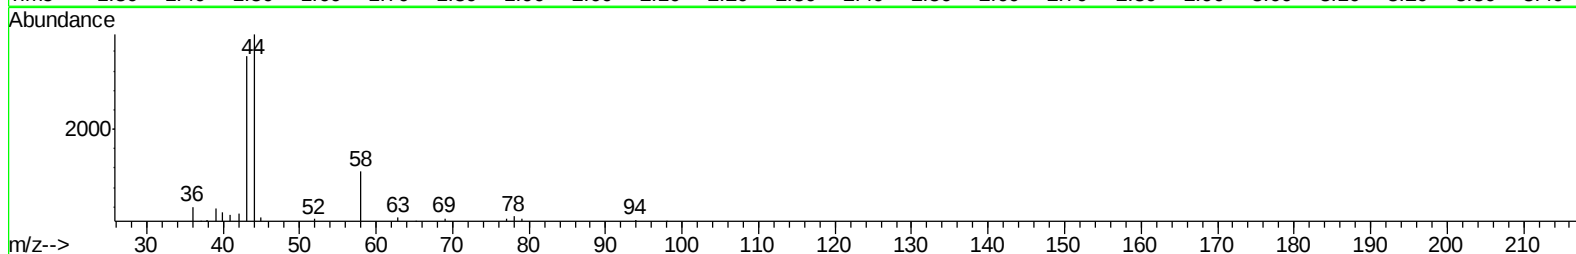


Data File : VU033806.D
Acq On : 15 Aug 2019 13:26
Operator : JC/SP
Sample : MDL05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 16 01:12:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR081419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 01:09:16 2019
Response via : Initial Calibration

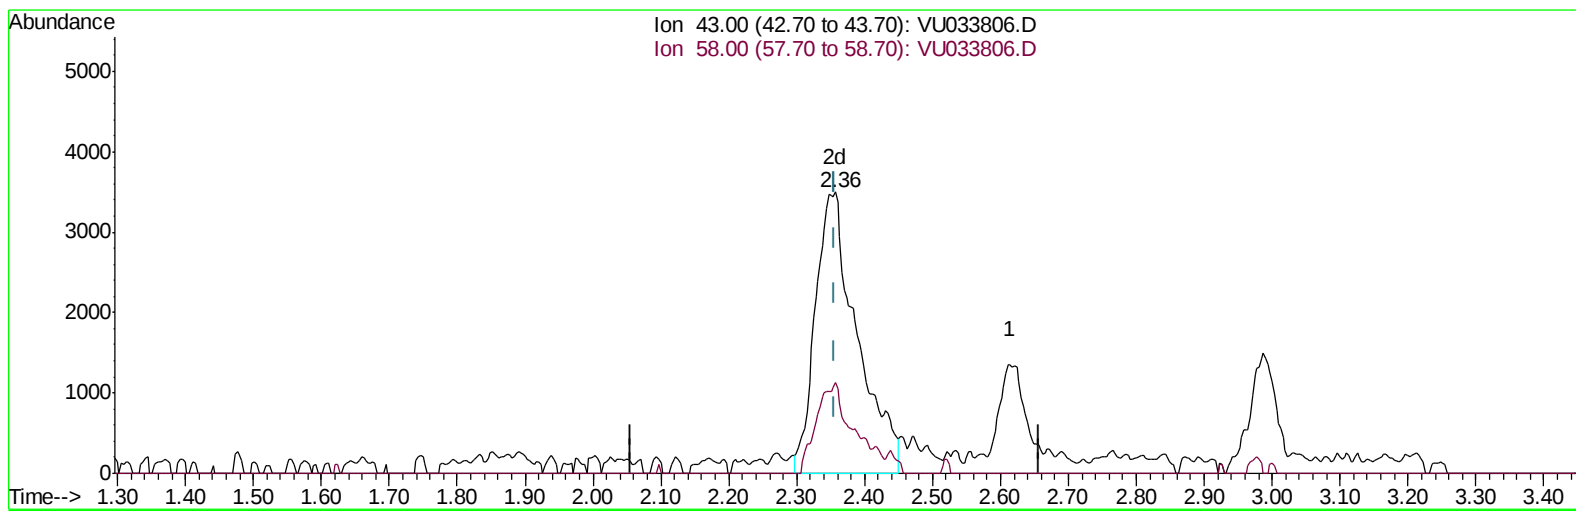

TIC: VU033806.D

(13) Acetone (T)

2.357min (+0.000) 3.59ug/L m

response 14958

Ion	Exp%	Act%
43.00	100	100
58.00	13.50	1.82
0.00	0.00	0.00
0.00	0.00	0.00