


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081519\
Data File : VU033801.D
Acq On : 15 Aug 2019 09:21
Operator : JC/SP
Sample : BFB01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR081419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Aug 16 01:09:16 2019

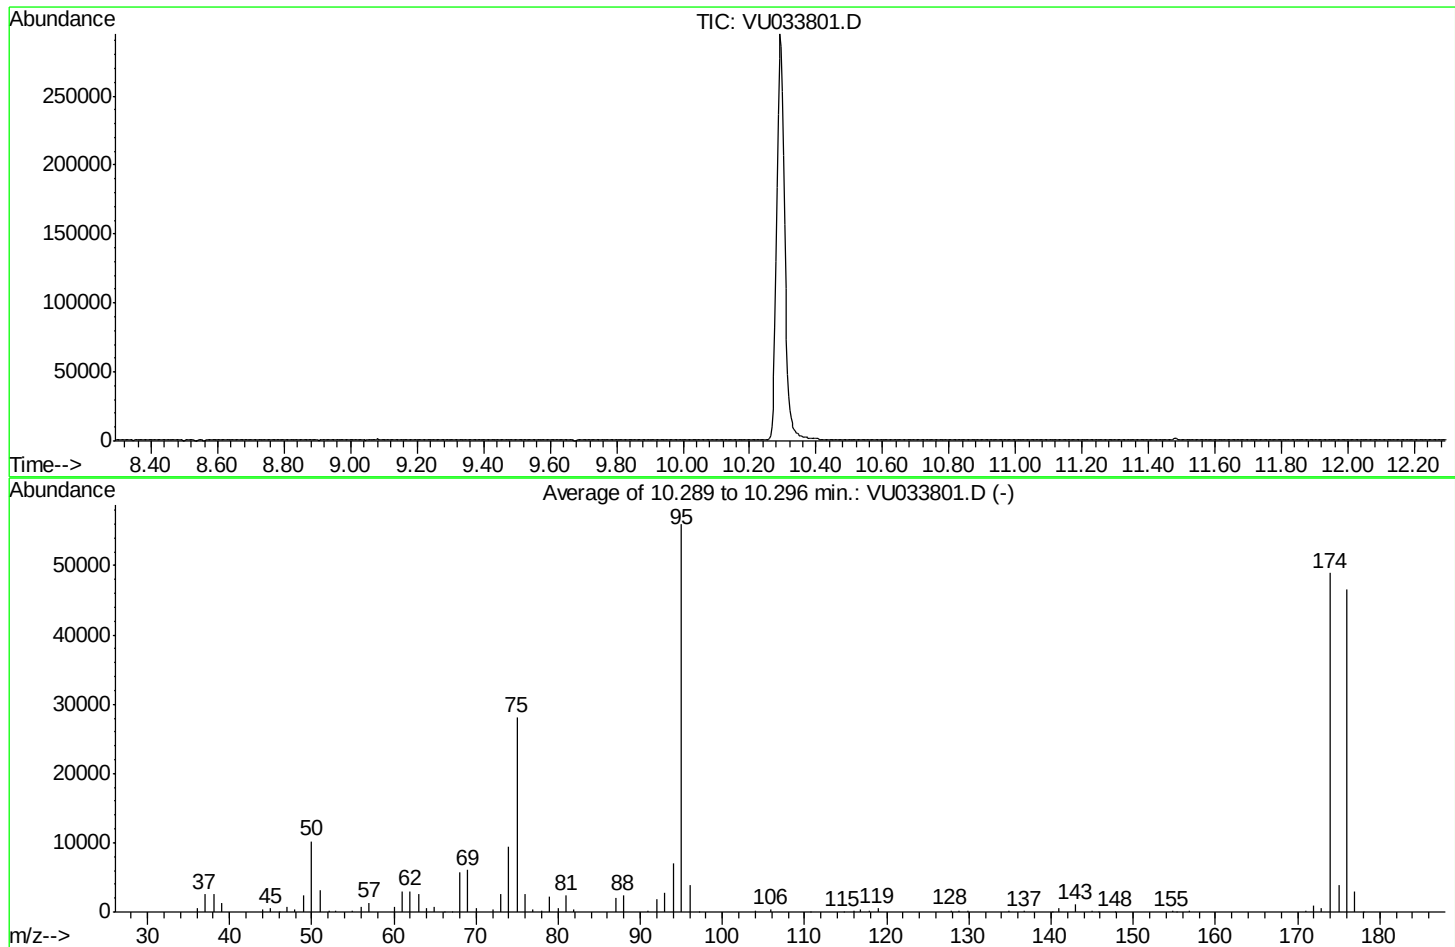

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	10232	PASS
75	95	30	80	50.1	28016	PASS
95	95	100	100	100.0	55973	PASS
96	95	5	9	7.1	3975	PASS
173	174	0.00	2	1.1	559	PASS
174	95	50	120	87.4	48909	PASS
175	174	5	9	8.1	3963	PASS
176	174	95	101	95.3	46586	PASS
177	176	5	9	6.2	2905	PASS

m/z	Abundance
36.10	490.0
37.00	2539.0
38.00	2656.0
39.00	1376.0
40.20	142.0
43.90	945.0
45.00	478.0
46.00	117.0
47.00	605.0
47.90	341.0
48.90	2480.0
50.00	9993.0
51.10	3005.0
52.00	166.0
52.90	198.0
55.00	319.0
55.90	815.0
57.00	1400.0
60.00	691.0
61.00	2744.0
62.00	2790.0
63.00	2664.0
64.00	446.0
64.90	647.0
67.00	106.0
68.00	5426.0
69.00	5832.0
70.00	521.0
72.10	416.0
73.00	2667.0
74.00	9253.0
75.00	27360.0
76.00	2536.0
76.90	340.0
78.00	245.0
78.90	2165.0
80.00	608.0
80.90	2477.0
81.90	342.0
86.90	2035.0
87.90	2340.0
91.00	149.0
92.00	1772.0
93.00	2569.0
94.00	6993.0
95.00	54776.0
96.00	3888.0
97.10	100.0
104.00	248.0
105.90	348.0
114.80	137.0
115.90	291.0
116.90	471.0
118.00	244.0
118.90	469.0
127.80	285.0
128.80	163.0
129.80	203.0
134.80	131.0
136.80	118.0
140.10	106.0
140.90	609.0
143.00	1000.0
144.90	239.0
147.80	132.0
154.80	156.0
156.90	112.0
171.90	983.0
174.00	46784.0
175.00	3894.0
176.00	44128.0
176.90	2818.0
178.00	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.10	465.0
37.00	2530.0
38.10	2344.0
39.00	1211.0
39.90	166.0
44.00	854.0
45.00	527.0
46.90	688.0
47.90	384.0
49.00	2097.0
50.00	10197.0
51.00	3362.0
52.10	249.0
53.00	130.0
54.90	164.0
56.00	819.0
57.00	1363.0
60.00	611.0
61.00	2934.0
62.00	3050.0
63.00	2606.0
64.00	502.0
65.00	769.0
66.20	101.0
68.00	5885.0
69.00	6164.0
70.00	517.0
72.10	341.0
73.00	2474.0
74.00	9257.0
75.00	27880.0
76.00	2432.0
77.00	389.0
77.90	267.0
78.90	2203.0
80.00	657.0
81.00	2228.0
81.90	399.0
87.00	2152.0
87.90	2272.0
90.90	202.0
92.00	1874.0
93.00	2813.0
94.00	6726.0
95.00	55224.0
96.00	3915.0
103.90	210.0
105.90	263.0
116.00	205.0
116.90	406.0
117.90	294.0
118.90	516.0
127.90	183.0
128.80	148.0
129.90	267.0
134.90	103.0
136.80	127.0
140.90	612.0
143.00	1023.0
145.00	274.0
145.70	101.0
154.80	147.0
155.20	107.0
156.90	132.0
171.00	230.0
171.90	1025.0
172.80	903.0
174.00	49632.0
175.00	3872.0
176.00	47504.0
176.90	2977.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.10	476.0
37.00	2681.0
38.00	2573.0
39.00	1336.0
40.00	119.0
44.00	914.0
45.00	510.0
46.00	103.0
46.90	725.0
47.90	359.0
49.00	2454.0
50.00	10506.0
51.10	3234.0
52.10	203.0
52.90	177.0
54.90	242.0
56.00	818.0
57.00	1412.0
60.00	690.0
61.00	3052.0
62.00	3036.0
63.00	2725.0
64.00	494.0
64.90	714.0
68.00	6058.0
69.00	6244.0
70.00	551.0
72.10	400.0
73.00	2639.0
74.00	9610.0
75.00	28808.0
76.00	2630.0
76.90	365.0
78.00	266.0
78.90	2275.0
80.00	678.0
80.90	2410.0
81.90	402.0
87.00	2154.0
87.90	2369.0
90.90	172.0
92.00	1960.0
93.00	2852.0
94.00	7307.0
95.00	57920.0
96.00	4124.0
103.90	216.0
105.90	331.0
110.70	106.0
114.70	129.0
115.90	233.0
116.80	464.0
118.00	286.0
118.90	528.0
127.80	257.0
128.80	168.0
129.80	245.0
134.90	140.0
136.80	147.0
140.90	646.0
143.00	1061.0
145.00	268.0
145.80	114.0
147.80	122.0
154.80	166.0
156.90	133.0
171.00	219.0
171.90	1032.0
172.90	775.0
174.00	50312.0
175.00	4123.0
176.00	48128.0
176.90	2920.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

Scan 2849 (10.251 min): VU033801.D
BFB01

m/z	Abundance
39.90	211.0
44.00	537.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01