


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081524\
Data File : VU060458.D
Acq On : 15 Aug 2024 09:00
Operator : MD/SY
Sample : BFB186
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB186

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Aug 16 04:55:30 2024

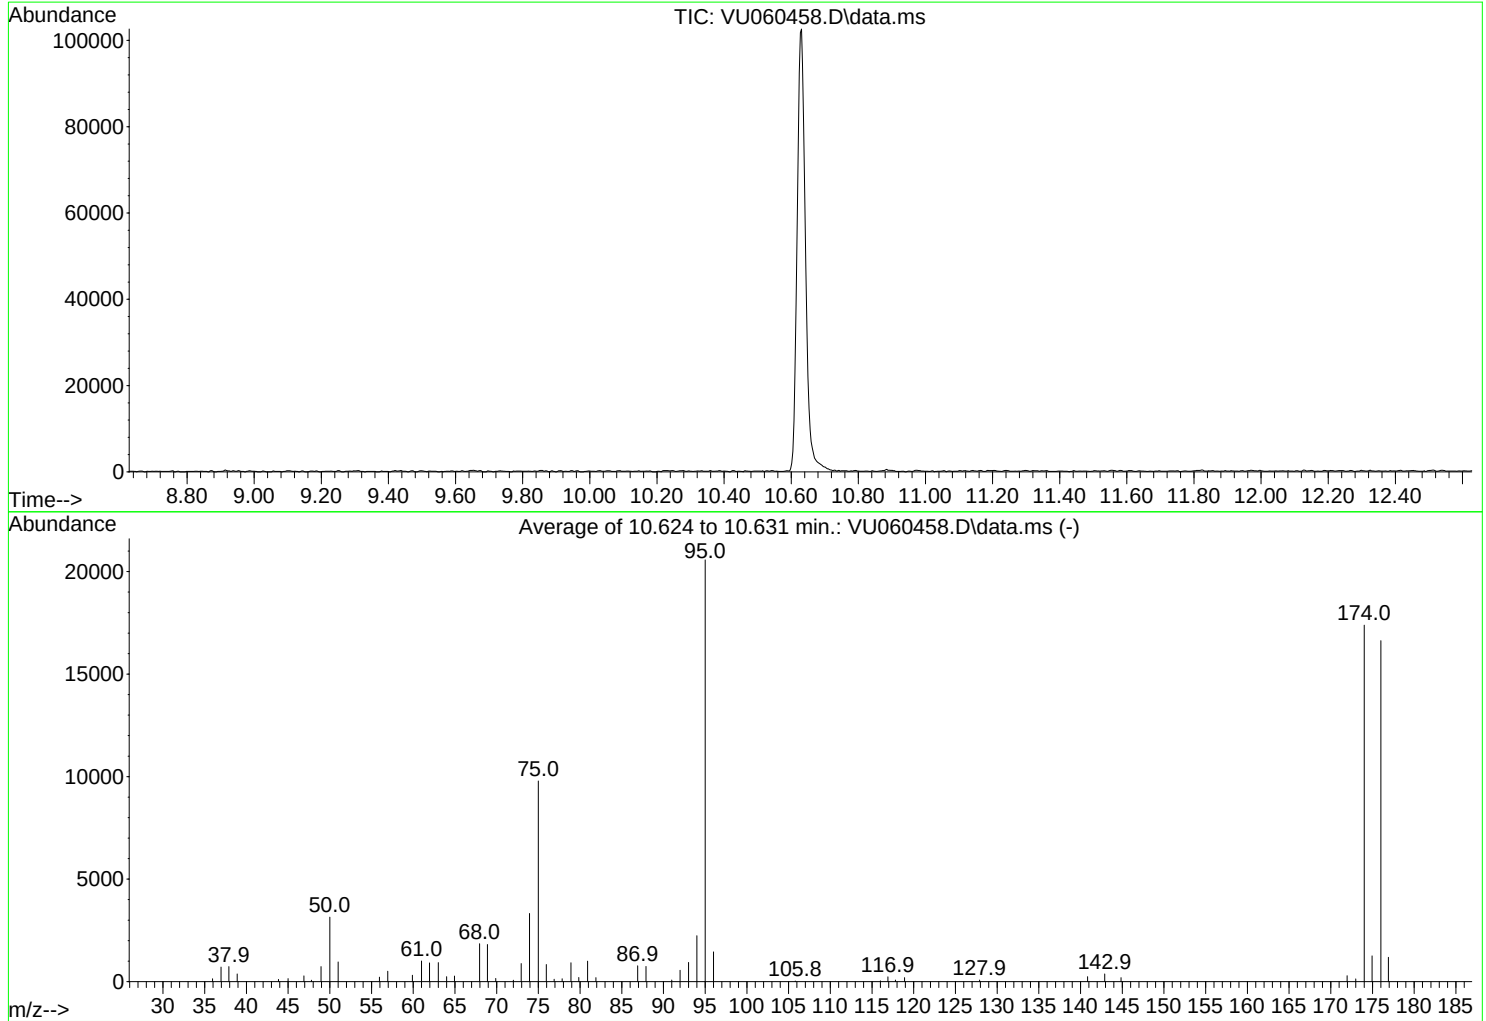

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	3147	PASS
75	95	30	80	47.6	9787	PASS
95	95	100	100	100.0	20573	PASS
96	95	5	9	7.1	1452	PASS
173	174	0.00	2	0.7	130	PASS
174	95	50	120	84.5	17389	PASS
175	174	5	9	7.2	1254	PASS
176	174	95	101	95.6	16631	PASS
177	176	5	9	7.1	1189	PASS

m/z	Abundance
39.90	113.0
43.80	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB186

m/z	Abundance
35.90	157.0
36.90	692.0
37.90	729.0
38.90	288.0
43.90	208.0
45.00	132.0
46.90	236.0
47.80	102.0
48.90	680.0
50.00	3009.0
51.00	893.0
56.00	204.0
57.00	459.0
59.90	284.0
61.00	947.0
62.00	788.0
63.00	817.0
64.00	211.0
64.90	293.0
67.90	1642.0
68.90	1726.0
69.90	175.0
73.00	808.0
74.00	3132.0
75.00	9574.0
75.90	800.0
76.90	113.0
77.80	128.0
78.90	886.0
79.80	214.0
80.90	970.0
81.90	183.0
86.90	772.0
87.90	648.0
92.00	539.0
93.00	860.0
94.00	2155.0
95.00	19536.0
96.00	1312.0
116.90	195.0
117.80	109.0
118.90	190.0
127.90	126.0
140.90	233.0
142.90	365.0
144.80	175.0
172.00	251.0
174.00	15855.0
174.90	1194.0
176.00	15390.0
176.90	1072.0

Instrument :
MSVOA_U
ClientSampleId :
BFB186

m/z	Abundance
35.90	148.0
36.90	716.0
37.90	761.0
38.90	398.0
43.90	265.0
45.00	145.0
46.90	301.0
47.80	114.0
48.90	743.0
50.00	3266.0
51.00	976.0
56.00	220.0
56.90	540.0
59.90	340.0
61.00	1027.0
61.90	924.0
63.00	954.0
64.00	260.0
64.90	272.0
68.00	1857.0
68.90	1867.0
69.90	156.0
72.00	104.0
73.00	899.0
74.00	3447.0
75.00	10046.0
76.00	832.0
76.90	123.0
77.80	154.0
78.90	950.0
79.80	207.0
80.90	1033.0
81.90	200.0
86.90	783.0
87.90	748.0
91.00	114.0
92.00	586.0
93.00	966.0
94.00	2329.0
95.00	21112.0
96.00	1497.0
116.90	244.0
117.80	117.0
118.90	197.0
127.90	116.0
140.90	260.0
142.90	387.0
144.90	202.0
172.00	308.0
174.00	17952.0
174.90	1275.0
176.00	17072.0
176.90	1243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB186

m/z	Abundance
36.00	125.0
37.00	728.0
37.90	708.0
38.90	434.0
43.90	272.0
45.00	164.0
46.90	301.0
49.00	780.0
50.00	3165.0
51.00	1018.0
55.90	221.0
57.00	527.0
59.90	323.0
61.00	1053.0
61.90	1020.0
63.00	1016.0
64.00	255.0
65.00	254.0
68.00	2043.0
68.90	1831.0
69.90	135.0
72.00	100.0
72.90	929.0
73.90	3398.0
75.00	9741.0
76.00	875.0
76.90	127.0
77.90	142.0
78.90	934.0
79.90	189.0
80.90	991.0
81.90	200.0
86.90	765.0
87.90	817.0
91.00	121.0
92.00	550.0
93.00	995.0
94.00	2243.0
95.00	21072.0
96.00	1547.0
105.80	102.0
116.00	111.0
116.90	254.0
118.90	188.0
140.80	238.0
142.90	368.0
144.90	204.0
171.90	315.0
173.00	389.0
174.00	18360.0
175.00	1293.0
176.00	17432.0
176.90	1251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB186