


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081618\
Data File : VU026171.D
Acq On : 16 Aug 2018 09:35
Operator : MD/SY
Sample : BFB48
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081518WMA.M
Title : VOC Analysis
Last Update : Thu Aug 16 16:15:16 2018

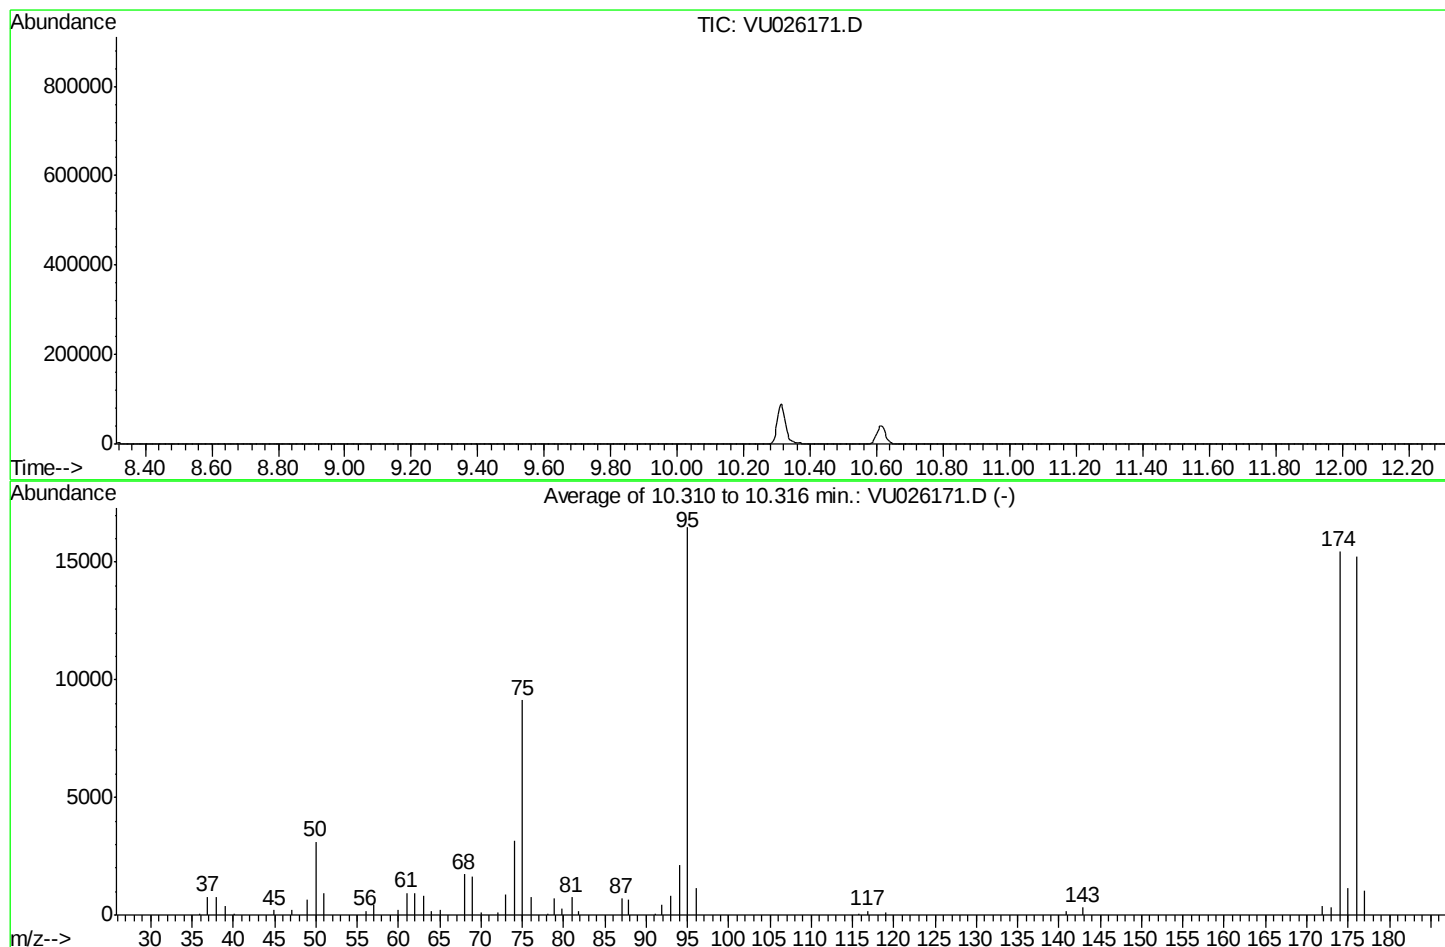

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	3131	PASS
75	95	30	80	55.4	9142	PASS
95	95	100	100	100.0	16488	PASS
96	95	5	9	6.8	1127	PASS
173	174	0.00	2	2.0	306	PASS
174	95	50	120	93.6	15436	PASS
175	174	5	9	7.4	1137	PASS
176	174	95	101	98.7	15238	PASS
177	176	5	9	6.7	1016	PASS

m/z	Abundance
43.90	404.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	100.0
36.90	780.0
38.00	841.0
39.00	437.0
40.10	136.0
44.00	392.0
45.00	191.0
47.00	256.0
49.00	716.0
50.00	3151.0
51.00	973.0
55.90	224.0
57.00	473.0
59.90	220.0
61.00	1022.0
62.00	906.0
63.00	795.0
63.90	142.0
65.00	231.0
67.90	1600.0
69.00	1703.0
70.00	129.0
72.00	110.0
73.00	999.0
74.00	3135.0
75.00	9357.0
76.00	776.0
78.90	649.0
79.80	249.0
81.00	775.0
81.90	171.0
87.00	717.0
87.90	689.0
92.00	394.0
93.00	886.0
94.00	2138.0
95.00	16672.0
96.00	1207.0
116.90	163.0
118.90	117.0
140.80	150.0
142.90	300.0
171.90	302.0
172.90	336.0
174.00	15679.0
175.00	1142.0
176.00	15219.0
176.90	988.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.90	780.0
38.00	771.0
39.10	346.0
40.10	110.0
44.00	310.0
44.90	209.0
47.10	219.0
49.00	719.0
50.00	3271.0
51.00	985.0
56.00	178.0
57.00	476.0
59.90	209.0
61.00	929.0
62.00	926.0
63.00	840.0
63.90	166.0
65.00	228.0
67.90	1798.0
69.00	1678.0
69.90	127.0
72.00	126.0
73.00	897.0
74.00	3247.0
75.00	9387.0
76.00	751.0
78.90	730.0
79.90	268.0
81.00	763.0
81.80	167.0
87.00	735.0
87.90	621.0
91.10	107.0
91.90	442.0
93.00	823.0
94.00	2203.0
95.00	16848.0
96.00	1153.0
115.70	109.0
116.90	194.0
118.90	110.0
140.90	181.0
142.90	335.0
171.80	400.0
172.90	339.0
174.00	15984.0
175.00	1153.0
176.00	15749.0
176.90	1025.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.90	758.0
38.00	610.0
39.00	345.0
43.90	330.0
44.90	195.0
47.10	197.0
48.90	598.0
50.00	2972.0
51.00	872.0
56.10	153.0
57.00	417.0
59.90	159.0
61.00	904.0
62.00	911.0
63.00	773.0
64.00	169.0
65.00	194.0
68.00	1781.0
69.00	1504.0
69.90	100.0
72.00	104.0
73.00	796.0
74.00	3071.0
75.00	8683.0
76.00	729.0
78.10	102.0
78.90	738.0
79.90	242.0
80.90	700.0
81.90	151.0
87.00	628.0
87.90	577.0
91.90	492.0
93.00	734.0
94.00	2085.0
95.00	15945.0
96.00	1022.0
115.80	101.0
116.80	191.0
119.00	116.0
140.90	234.0
142.90	307.0
171.90	461.0
172.90	244.0
174.00	14646.0
175.00	1116.0
176.00	14746.0
176.90	1037.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48