


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081619\
 Data File : VU033808.D
 Acq On : 15 Aug 2019 14:14
 Operator : JC/SP
 Sample : BFB57
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB57

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 17 02:15:05 2019

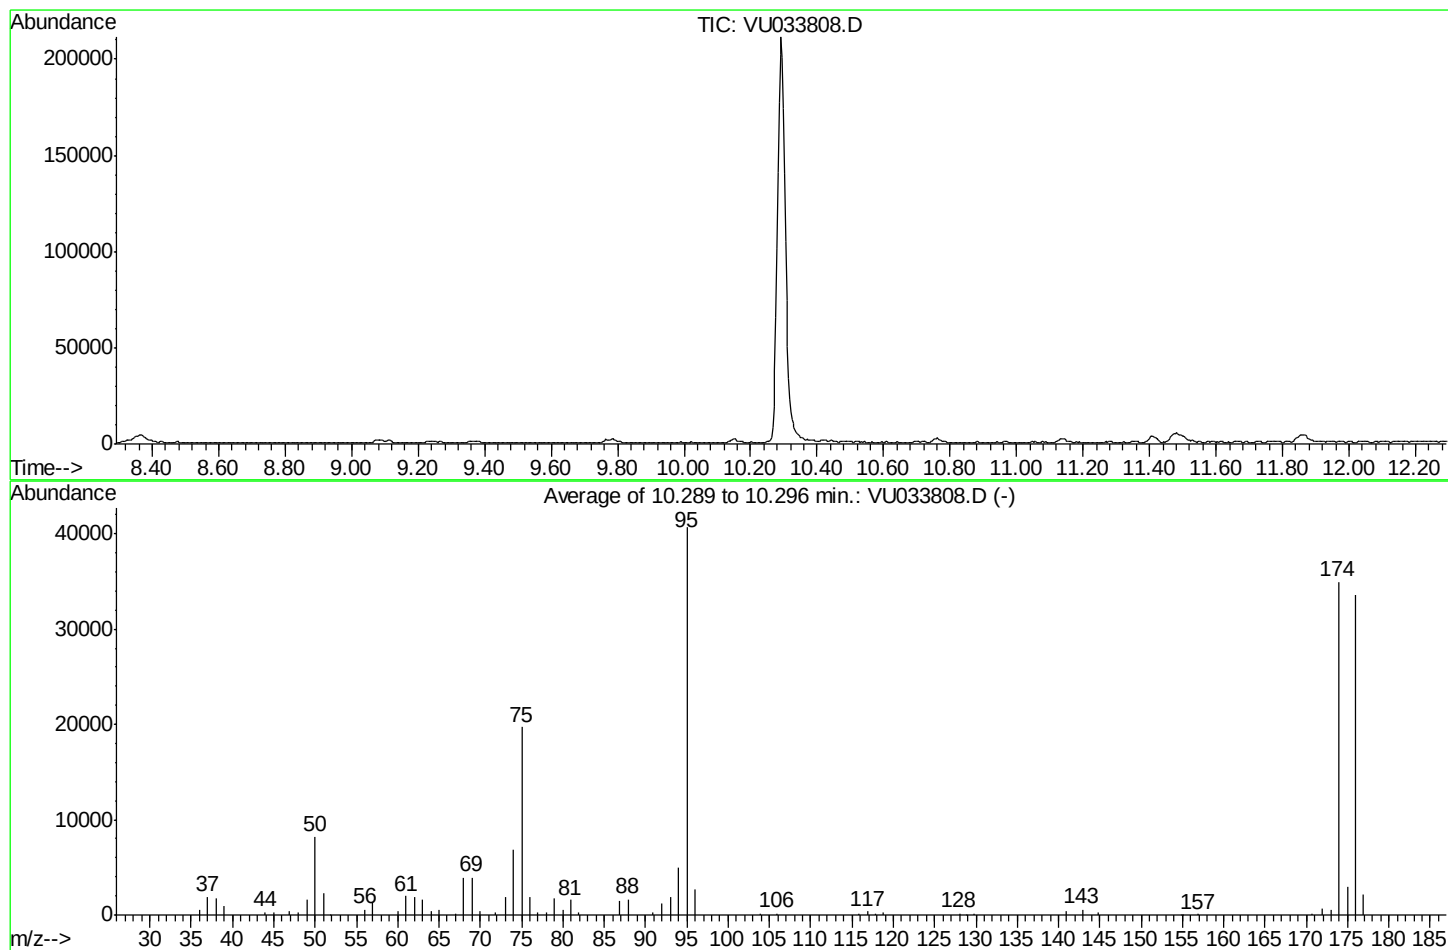

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	8200	PASS
75	95	30	80	48.5	19733	PASS
95	95	100	100	100.0	40674	PASS
96	95	5	9	6.6	2668	PASS
173	174	0.00	2	1.6	547	PASS
174	95	50	120	86.0	34986	PASS
175	174	5	9	8.3	2900	PASS
176	174	95	101	96.1	33626	PASS
177	176	5	9	6.5	2197	PASS

m/z	Abundance
35.90	507.0
37.00	1892.0
38.00	1856.0
39.00	998.0
40.00	383.0
44.00	948.0
45.00	282.0
46.80	362.0
48.00	248.0
49.10	1615.0
50.00	8265.0
51.10	2367.0
51.90	107.0
56.10	619.0
57.00	1232.0
60.00	403.0
61.00	2115.0
62.00	1826.0
63.10	1593.0
64.00	329.0
65.10	570.0
67.10	160.0
68.00	3934.0
69.00	3853.0
69.90	418.0
71.80	205.0
73.00	1850.0
74.10	6749.0
75.00	19448.0
76.10	1959.0
77.00	193.0
77.90	255.0
78.90	1782.0
80.00	548.0
80.90	1456.0
81.80	289.0
86.90	1461.0
87.90	1828.0
90.80	229.0
92.00	1183.0
93.00	1947.0
94.00	4723.0
95.00	40976.0
96.00	2726.0
103.90	184.0
105.90	128.0
115.80	203.0
116.90	416.0
117.90	224.0
118.80	258.0
128.00	185.0
129.90	151.0
140.90	431.0
142.90	487.0
144.90	224.0
157.00	102.0
171.90	635.0
173.90	34008.0
175.00	2699.0
175.90	33016.0
176.90	2228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
35.90	504.0
37.00	1988.0
38.00	1842.0
39.00	988.0
40.00	418.0
44.00	897.0
45.00	279.0
46.90	412.0
48.00	303.0
49.10	1651.0
50.00	8488.0
51.10	2421.0
51.90	100.0
56.10	617.0
57.00	1410.0
60.00	383.0
61.00	2055.0
62.00	1848.0
63.10	1577.0
64.00	364.0
65.00	614.0
67.00	154.0
68.00	3958.0
69.00	4055.0
69.90	400.0
71.90	266.0
73.00	1973.0
74.10	7087.0
75.00	20376.0
76.00	1935.0
76.90	228.0
78.00	315.0
78.90	1806.0
80.00	539.0
80.90	1614.0
81.90	267.0
86.90	1487.0
87.90	1772.0
90.90	228.0
92.00	1194.0
93.00	2012.0
94.00	5062.0
95.00	41920.0
96.00	2749.0
103.90	176.0
106.00	176.0
115.80	223.0
117.00	420.0
117.90	222.0
118.80	315.0
128.00	171.0
128.90	102.0
129.70	160.0
140.90	423.0
142.90	563.0
144.90	251.0
154.80	109.0
156.90	111.0
170.80	118.0
171.90	729.0
173.00	813.0
173.90	36176.0
174.90	3023.0
175.90	34472.0
176.90	2257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
36.00	419.0
37.00	1873.0
38.00	1701.0
39.00	848.0
40.00	415.0
44.00	851.0
45.00	209.0
47.00	479.0
48.00	306.0
49.00	1657.0
50.00	7847.0
51.10	2205.0
56.00	590.0
57.00	1324.0
60.00	314.0
61.00	1744.0
62.00	1864.0
63.00	1529.0
64.00	387.0
65.00	566.0
67.00	120.0
68.00	3741.0
69.00	3927.0
70.00	376.0
71.90	313.0
73.00	1810.0
74.00	6721.0
75.00	19376.0
76.00	1741.0
76.90	232.0
78.00	295.0
78.90	1617.0
80.00	429.0
80.90	1598.0
81.90	253.0
86.90	1520.0
87.90	1427.0
90.90	190.0
92.00	1171.0
93.00	1831.0
94.00	4972.0
95.00	39128.0
96.00	2531.0
103.80	146.0
106.00	246.0
115.80	187.0
116.90	319.0
117.80	160.0
118.80	339.0
128.00	136.0
128.80	105.0
129.70	180.0
140.90	393.0
142.90	645.0
144.80	277.0
155.00	105.0
156.90	108.0
170.70	149.0
172.00	798.0
173.00	830.0
173.90	34776.0
174.90	2980.0
175.90	33392.0
177.00	2108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

Scan 2850 (10.254 min): VU033808.D
BFB57

m/z	Abundance
40.00	786.0
43.90	616.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57