

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081621\
 Data File : VU044432.D
 Acq On : 16 Aug 2021 14:58
 Operator : SY/MD
 Sample : VU0816WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK001

Quant Time: Aug 17 03:02:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 17 02:56:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	5762	0.500	ug/L	0.02
5) Chlorobenzene-d5	9.361	117	5409	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.758	152	2703	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.605	65	3857	0.512	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.679	65	4105	0.474	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
7) 1,2-Dichloropropane-d6	6.639	67	3467	0.522	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.845	98	7390	0.486	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.696	84	2909	0.516	ug/L	0.02
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.701	75	40	0.053	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081621\
Data File : VU044432.D
Acq On : 16 Aug 2021 14:58
Operator : SY/MD
Sample : VU0816WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK001

Quant Time: Aug 17 03:02:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 17 02:56:51 2021
Response via : Initial Calibration

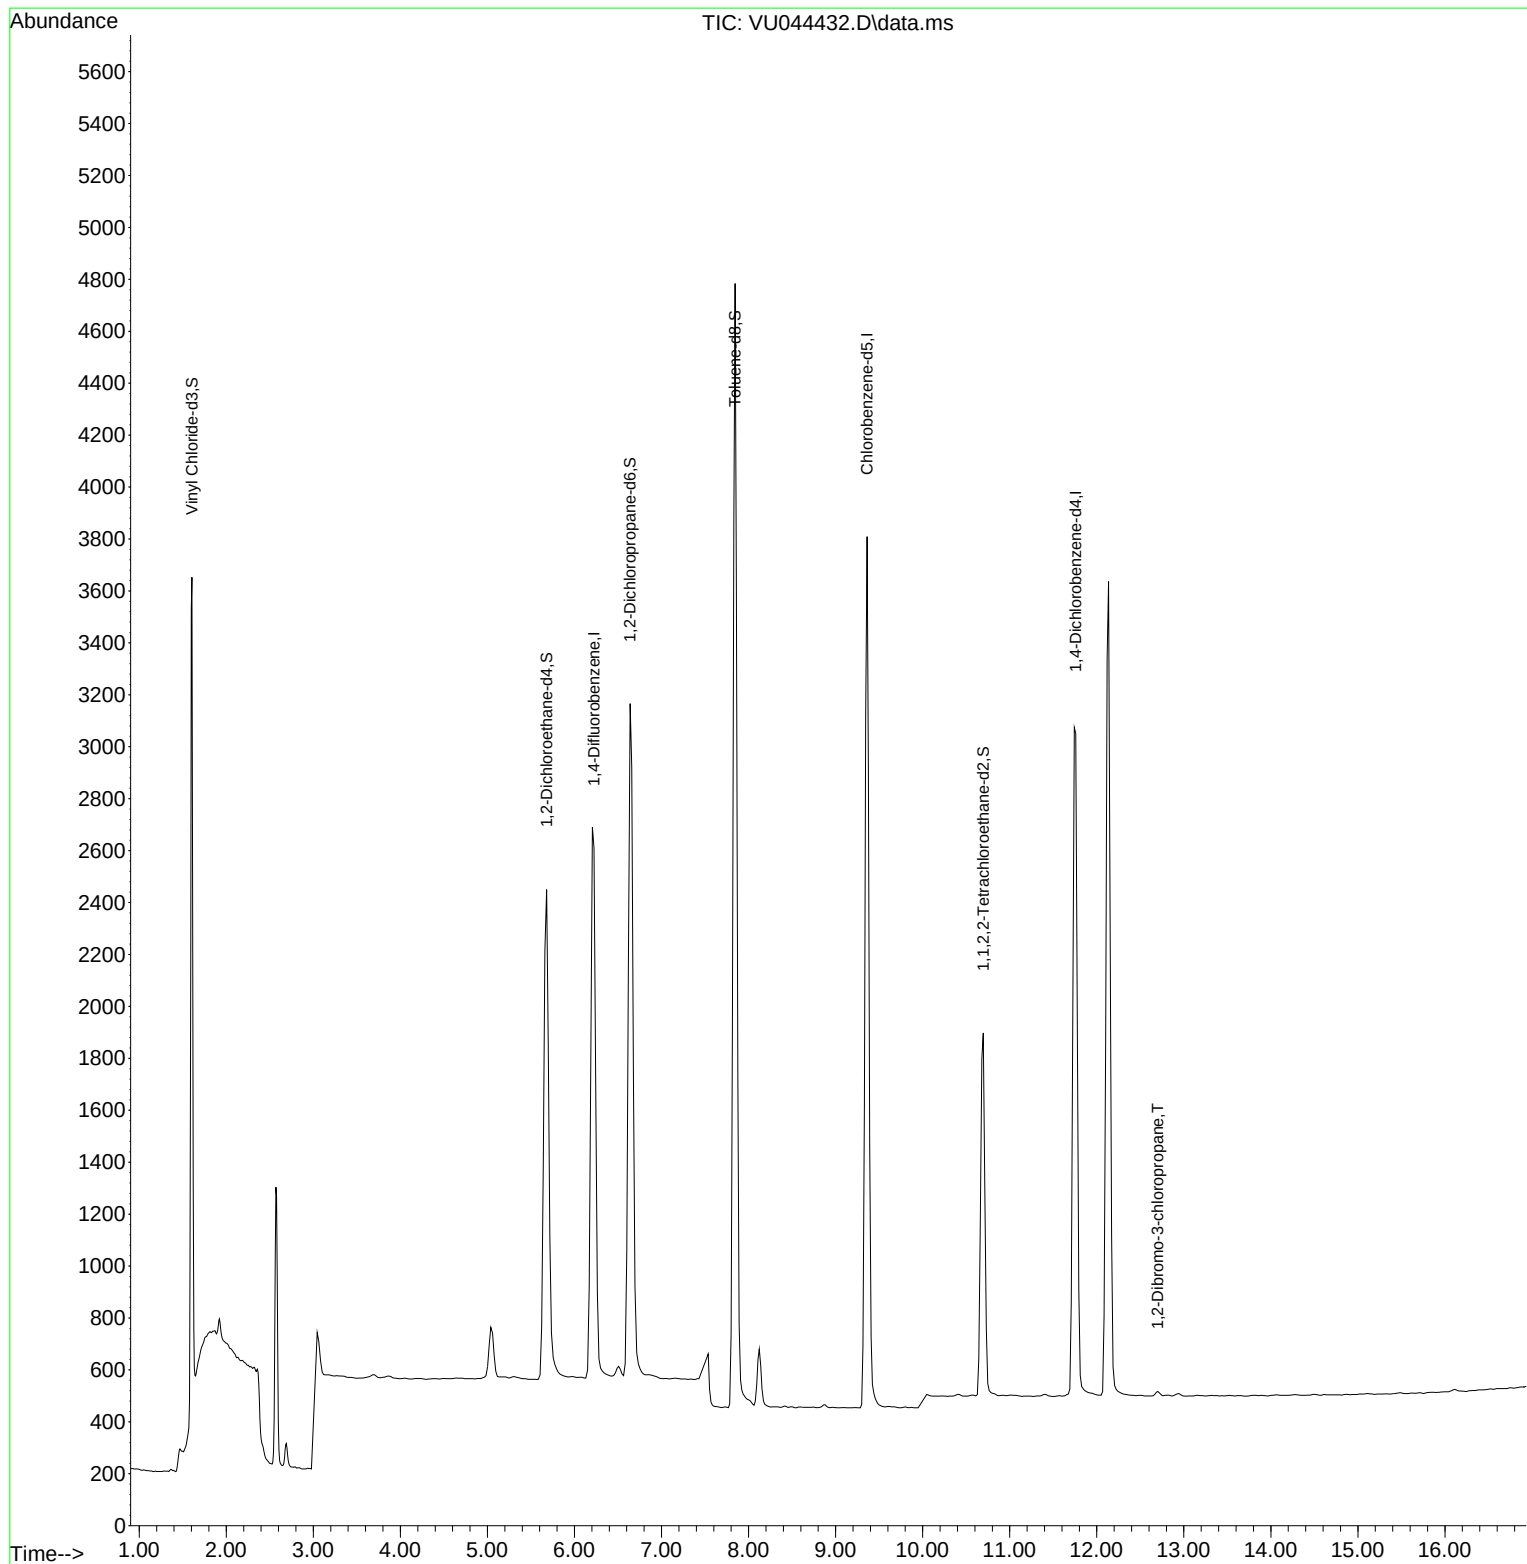

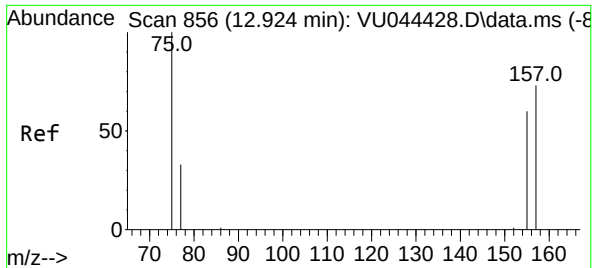

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.053 ug/L
 RT: 12.701 min Scan# 843
 Delta R.T. -0.223 min
 Lab File: VU044432.D
 Acq: 16 Aug 2021 14:58

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK001

Tgt Ion:	75	Resp:	40
Ion	Ratio	Lower	Upper
75	100		
157	75.0	63.5	95.3
155	78.1	56.2	84.4

