


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081621\
Data File : VU044425.D
Acq On : 16 Aug 2021 08:57
Operator : SY/MD
Sample : BFB002
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB002

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081621.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 17 02:56:51 2021

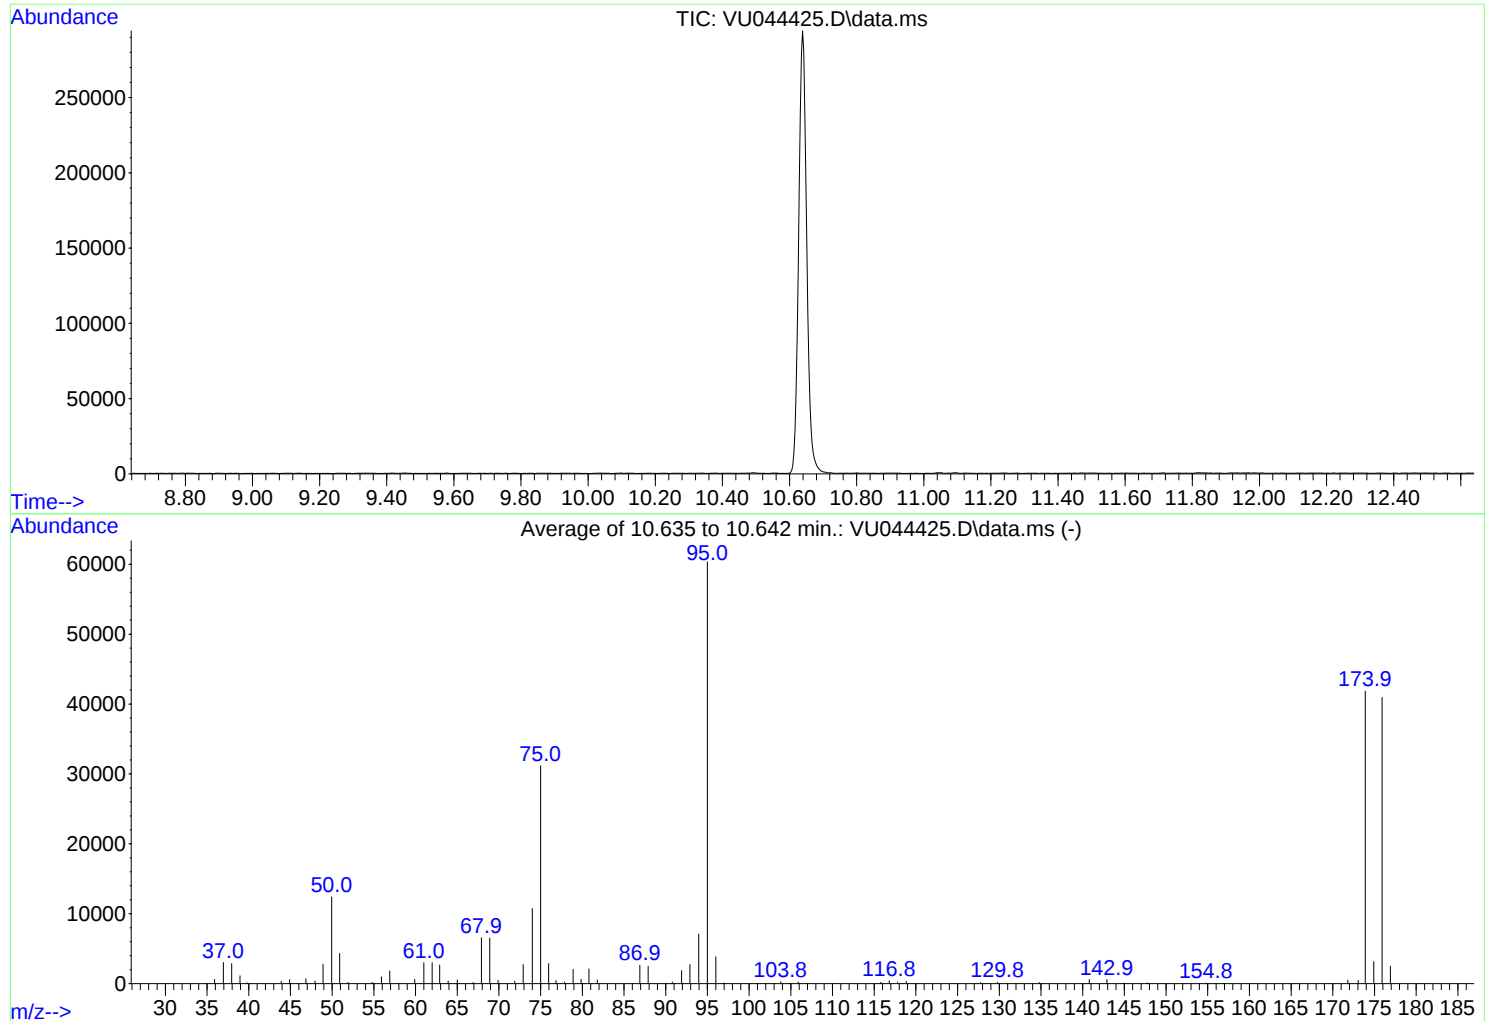

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	12404	PASS
75	95	30	80	51.7	31184	PASS
95	95	100	100	100.0	60344	PASS
96	95	5	9	6.4	3851	PASS
173	174	0.00	2	1.1	455	PASS
174	95	50	120	69.4	41851	PASS
175	174	5	9	7.6	3167	PASS
176	174	95	101	97.9	40957	PASS
177	176	5	9	6.1	2497	PASS

m/z	Abundance
43.90	313.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.90	589.0
37.00	3039.0
37.90	2998.0
38.90	1158.0
39.80	109.0
43.90	655.0
44.90	568.0
46.90	761.0
47.90	413.0
48.90	2826.0
50.00	12270.0
50.90	4317.0
51.90	173.0
54.80	172.0
55.90	938.0
56.90	1802.0
57.90	111.0
59.90	619.0
61.00	3087.0
62.00	2835.0
62.90	2687.0
63.90	323.0
65.00	513.0
66.90	132.0
67.90	6435.0
68.90	6609.0
69.90	483.0
71.90	316.0
72.90	2589.0
74.00	10525.0
75.00	30888.0
75.90	2759.0
76.80	400.0
77.90	261.0
78.90	1920.0
79.80	620.0
80.80	2014.0
81.80	450.0
86.90	2639.0
87.90	2491.0
90.80	191.0
91.90	1845.0
92.90	2585.0
94.00	6972.0
95.00	58920.0
96.00	3909.0
97.00	161.0
103.80	254.0
105.90	247.0
115.80	188.0
116.80	403.0
117.80	216.0
118.90	357.0
127.70	179.0
129.80	178.0
134.80	203.0
140.80	524.0
142.90	530.0
144.90	131.0
147.80	113.0
171.80	485.0
173.00	410.0
173.90	40448.0
174.90	3165.0
175.90	38992.0
176.90	2379.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.90	668.0
37.00	3138.0
38.00	2912.0
38.90	1141.0
39.80	117.0
43.90	676.0
44.90	594.0
45.80	105.0
46.80	752.0
48.00	407.0
48.90	2904.0
50.00	12775.0
50.90	4482.0
51.90	192.0
54.80	185.0
55.90	1030.0
56.90	1871.0
59.90	642.0
61.00	3060.0
62.00	3099.0
62.90	2748.0
63.90	372.0
65.00	566.0
66.90	183.0
67.90	6790.0
68.90	6703.0
69.90	471.0
71.90	345.0
72.90	2788.0
74.00	11070.0
75.00	32136.0
76.00	2924.0
76.80	451.0
77.90	245.0
78.90	2119.0
79.80	657.0
80.80	2178.0
81.80	548.0
86.90	2721.0
87.90	2588.0
90.80	229.0
91.90	1951.0
92.90	2820.0
94.00	7258.0
95.00	62344.0
96.00	3963.0
97.00	143.0
103.80	274.0
105.90	258.0
115.80	197.0
116.80	436.0
117.80	236.0
118.90	328.0
127.70	155.0
129.80	190.0
134.80	175.0
140.80	578.0
142.90	587.0
144.90	112.0
147.80	120.0
154.80	105.0
171.80	539.0
173.10	491.0
173.90	43112.0
174.90	3286.0
175.90	42368.0
176.90	2582.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.90	621.0
36.90	2867.0
37.90	2658.0
39.00	1044.0
39.80	129.0
43.90	643.0
44.90	558.0
46.80	650.0
48.00	340.0
48.90	2633.0
49.90	12168.0
50.90	4217.0
51.90	174.0
54.80	187.0
55.90	1023.0
56.90	1775.0
59.90	609.0
61.00	2849.0
62.00	3031.0
62.90	2513.0
63.90	396.0
65.00	518.0
66.90	198.0
67.90	6485.0
68.90	6264.0
69.90	425.0
71.90	360.0
72.90	2783.0
74.00	10591.0
75.00	30528.0
76.00	2884.0
76.90	441.0
77.80	216.0
78.90	2080.0
79.90	605.0
80.80	2148.0
81.80	600.0
86.90	2506.0
87.90	2435.0
90.80	264.0
91.90	1823.0
92.90	2774.0
93.90	7054.0
95.00	59768.0
96.00	3680.0
103.80	265.0
105.90	253.0
115.80	217.0
116.80	408.0
117.80	218.0
118.80	280.0
127.80	144.0
129.80	191.0
134.80	109.0
140.80	584.0
142.90	595.0
147.70	115.0
154.80	126.0
156.90	101.0
171.80	522.0
173.10	463.0
173.90	41992.0
174.90	3050.0
175.90	41512.0
176.90	2530.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002