
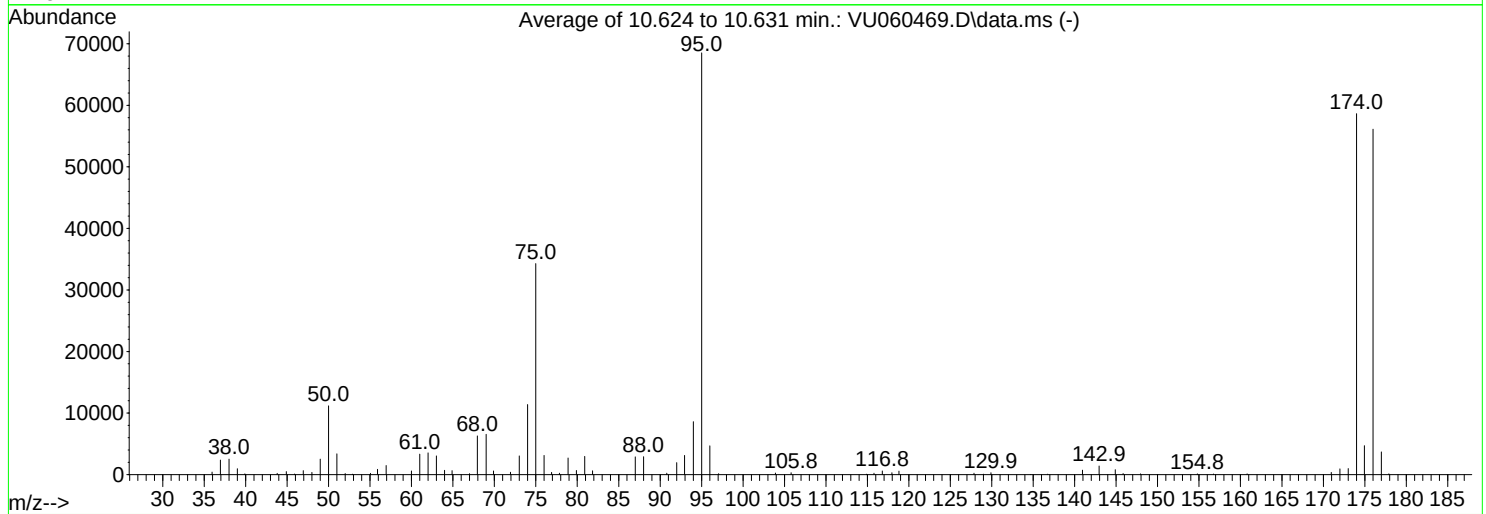


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081624\
Data File : VU060469.D
Acq On : 16 Aug 2024 11:16
Operator : MD/SY
Sample : BFB011
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB011

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 17 05:03:57 2024

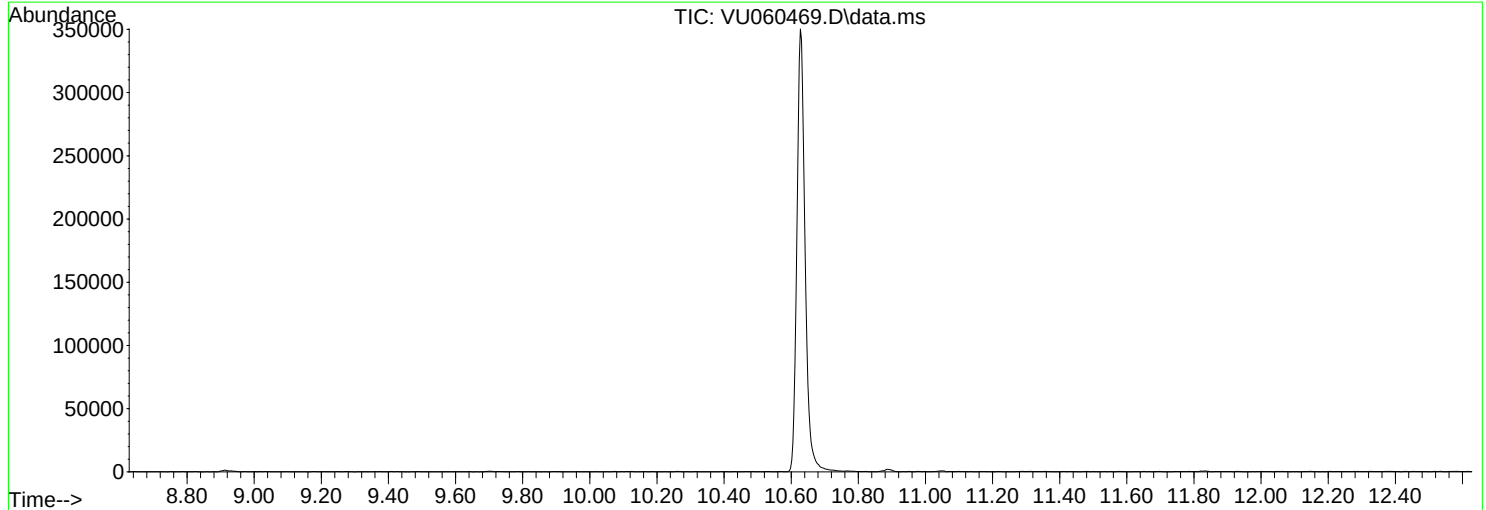

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	11174	PASS
75	95	30	80	50.0	34277	PASS
95	95	100	100	100.0	68520	PASS
96	95	5	9	6.9	4695	PASS
173	174	0.00	2	1.7	977	PASS
174	95	50	120	85.6	58632	PASS
175	174	5	9	8.0	4719	PASS
176	174	95	101	95.7	56117	PASS
177	176	5	9	6.6	3705	PASS

m/z	Abundance
43.80	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	400.0
37.00	2265.0
38.00	2502.0
39.00	956.0
40.00	121.0
43.90	422.0
44.90	568.0
45.90	106.0
46.90	679.0
48.00	328.0
49.00	2391.0
50.00	10763.0
51.00	3165.0
52.00	180.0
52.90	124.0
55.10	187.0
55.90	779.0
57.00	1613.0
60.00	547.0
61.00	3246.0
62.00	3617.0
63.00	2732.0
64.00	652.0
64.90	620.0
67.00	162.0
67.90	6162.0
69.00	6339.0
69.90	562.0
72.00	378.0
73.00	2890.0
74.00	10950.0
75.00	33384.0
76.00	3070.0
76.90	419.0
77.80	210.0
78.90	2652.0
79.90	641.0
80.90	2777.0
81.90	612.0
87.00	2860.0
88.00	2900.0
90.80	192.0
92.00	1904.0
93.00	2785.0
94.00	8280.0
95.00	66344.0
96.00	4661.0
97.00	140.0
103.90	266.0
105.80	314.0
114.90	108.0
115.80	256.0
116.80	564.0
117.90	334.0
118.80	509.0
127.90	222.0
129.90	311.0
134.70	108.0
136.80	112.0
140.90	680.0
142.90	1403.0
144.90	821.0
145.90	194.0
147.90	125.0
154.70	139.0
156.80	105.0
160.80	129.0
170.90	368.0
172.00	827.0
173.00	952.0
174.00	55168.0
174.90	4513.0
176.00	52696.0
177.00	3693.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
36.00	422.0
36.90	2474.0
38.00	2644.0
39.00	973.0
39.80	128.0
43.80	398.0
44.90	519.0
45.90	102.0
46.90	650.0
48.00	376.0
49.00	2566.0
50.00	11573.0
51.00	3498.0
52.00	188.0
52.90	107.0
55.00	221.0
55.90	906.0
57.00	1483.0
60.00	623.0
61.00	3417.0
62.00	3669.0
63.00	3152.0
64.00	724.0
64.90	667.0
67.00	150.0
68.00	6462.0
69.00	6780.0
69.90	619.0
72.00	408.0
73.00	3130.0
74.00	11763.0
75.00	35560.0
76.00	3249.0
76.90	369.0
77.80	234.0
78.90	2756.0
79.90	701.0
80.90	3067.0
81.80	655.0
87.00	2983.0
88.00	2997.0
90.80	230.0
92.00	2012.0
93.00	3247.0
94.00	8901.0
95.00	70728.0
96.00	4865.0
97.10	165.0
103.90	265.0
105.80	322.0
114.90	124.0
115.80	249.0
116.80	595.0
117.90	306.0
118.80	597.0
127.90	225.0
129.00	109.0
129.90	325.0
136.70	113.0
141.00	765.0
142.90	1472.0
144.90	850.0
145.90	174.0
148.00	146.0
154.80	125.0
156.80	120.0
160.80	130.0
170.90	364.0
172.00	985.0
173.00	990.0
174.00	60568.0
175.00	4818.0
176.00	58064.0
177.00	3768.0
177.90	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
36.00	422.0
36.90	2359.0
38.00	2418.0
39.00	994.0
39.90	122.0
43.90	373.0
44.90	420.0
45.90	100.0
47.00	610.0
48.00	387.0
49.00	2583.0
50.00	11186.0
51.00	3451.0
52.00	162.0
55.00	240.0
55.90	910.0
56.90	1352.0
60.00	598.0
61.00	3302.0
62.00	3288.0
63.00	3267.0
64.00	757.0
64.90	668.0
67.00	144.0
67.90	6244.0
69.00	6525.0
69.90	587.0
71.90	358.0
73.00	3123.0
74.00	11483.0
75.00	33888.0
76.00	3066.0
76.90	310.0
77.90	280.0
78.90	2668.0
79.90	681.0
80.90	3081.0
81.80	600.0
87.00	2850.0
88.00	2838.0
90.80	249.0
92.00	1962.0
92.90	3340.0
94.00	8642.0
95.00	68488.0
96.00	4558.0
97.00	151.0
103.90	243.0
105.80	337.0
115.80	213.0
116.80	615.0
118.00	270.0
118.80	647.0
127.80	243.0
129.00	108.0
129.90	316.0
141.00	734.0
143.00	1381.0
144.90	762.0
145.80	169.0
148.00	154.0
150.00	100.0
154.90	147.0
156.70	107.0
160.80	116.0
171.00	345.0
172.00	1012.0
173.00	990.0
174.00	60160.0
175.00	4826.0
176.00	57592.0
177.00	3654.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011