

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081718\
 Data File : VU026195.D
 Acq On : 17 Aug 2018 21:49
 Operator : MD/SY
 Sample : J4515-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0363

Quant Time: Aug 18 02:02:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 18 01:29:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	119956	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	121329	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	52843	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	35656	5.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.60%
7) Chloroethane-d5	1.68	69	28806	5.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.80%
11) 1,1-Dichloroethene-d2	2.27	63	54155	4.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.60%
20) 2-Butanone-d5	4.20	46	104789	57.93	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.86%
24) Chloroform-d	4.65	84	79221	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.80%
26) 1,2-Dichloroethane-d4	5.32	65	44433	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.40%
32) Benzene-d6	5.35	84	150992	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
36) 1,2-Dichloropropane-d6	6.34	67	50387	5.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.40%
41) Toluene-d8	7.57	98	131443	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
43) trans-1,3-Dichloropropene-	7.86	79	18243	5.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.60%
46) 2-Hexanone-d5	8.32	63	78687	52.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.12%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	39850	5.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	53255	5.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.20%


Target Compounds					Ovalue
13) Acetone	2.33	43	3117	2.60 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081718\
Data File : VU026195.D
Acq On : 17 Aug 2018 21:49
Operator : MD/SY
Sample : J4515-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0363

Quant Time: Aug 18 02:02:49 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 18 01:29:07 2018
Response via : Initial Calibration

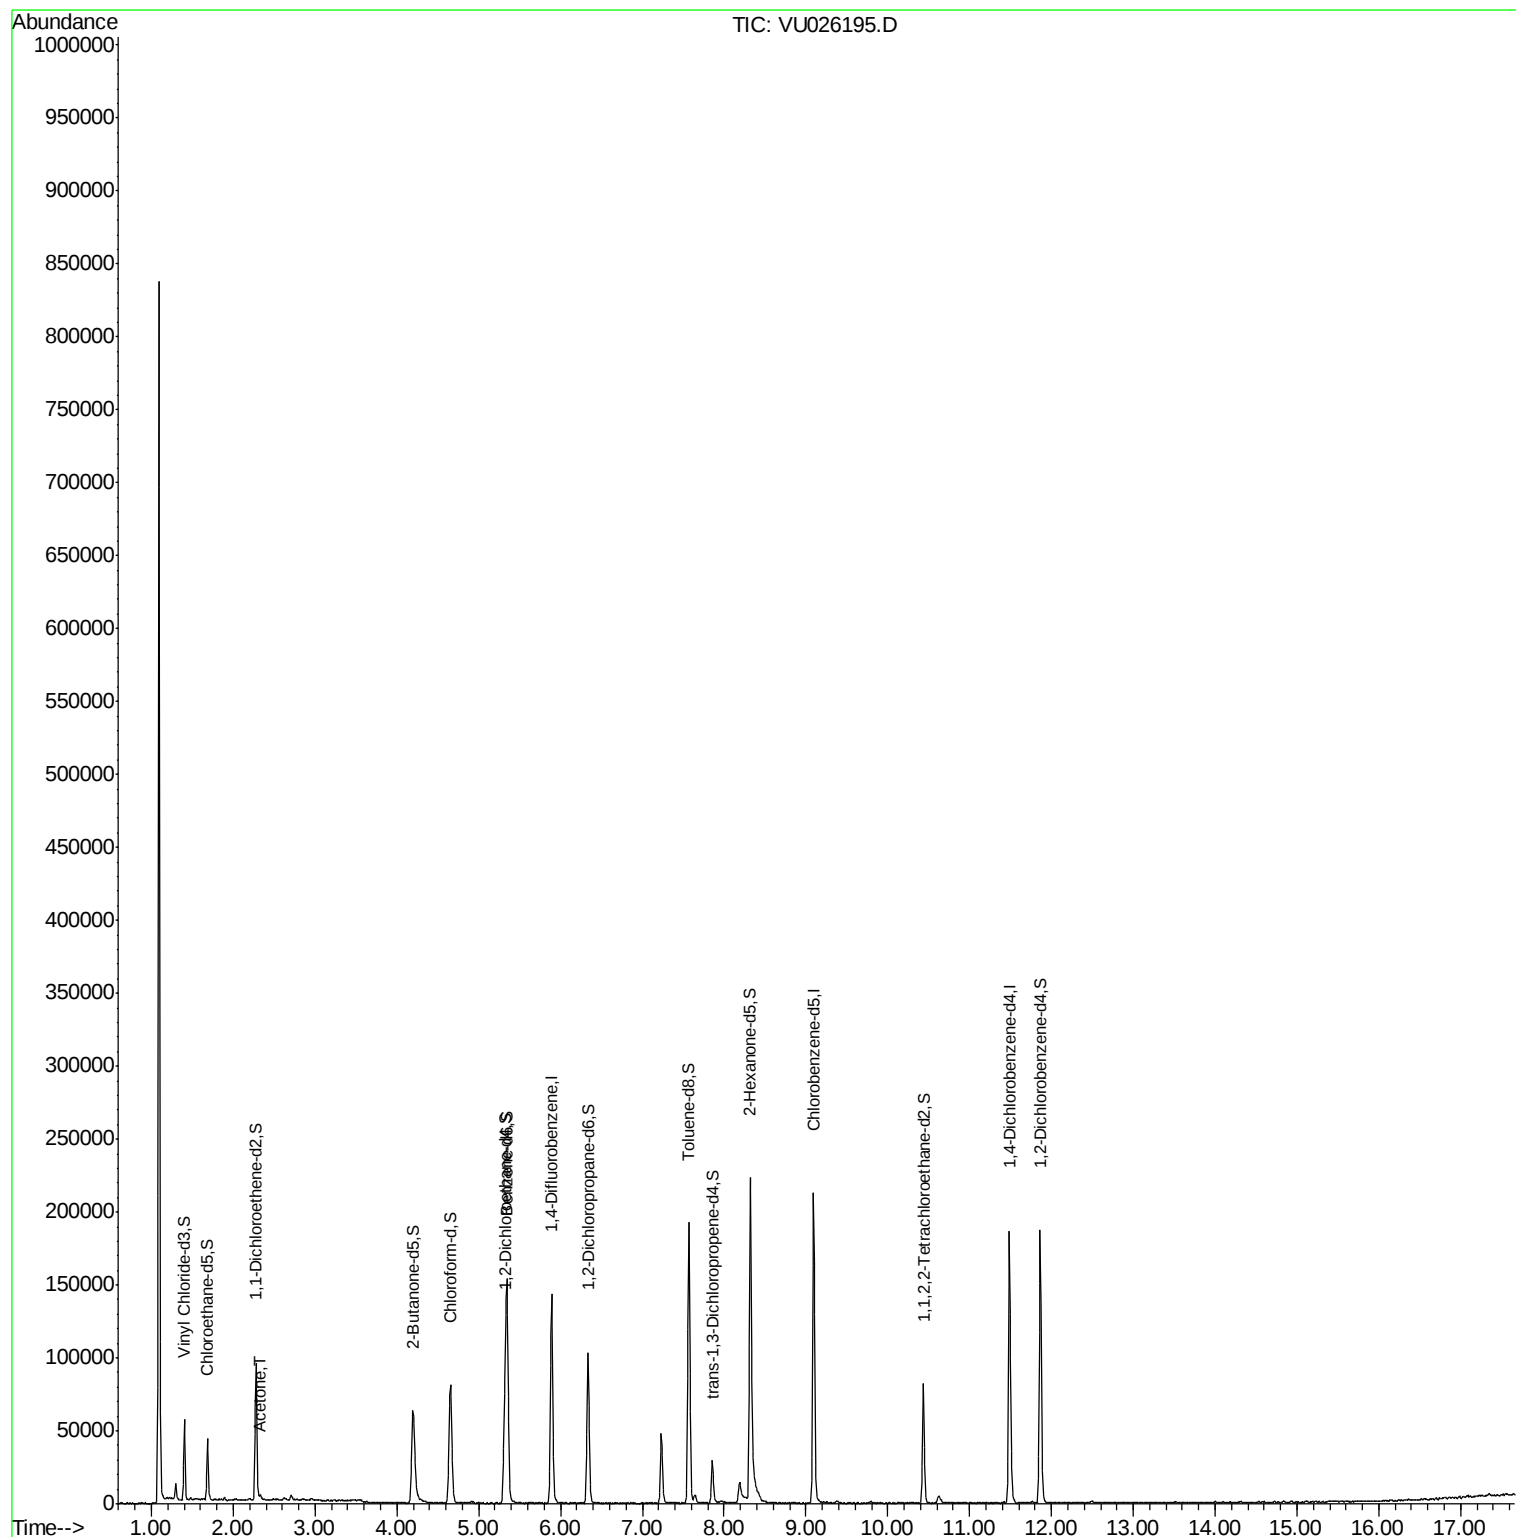

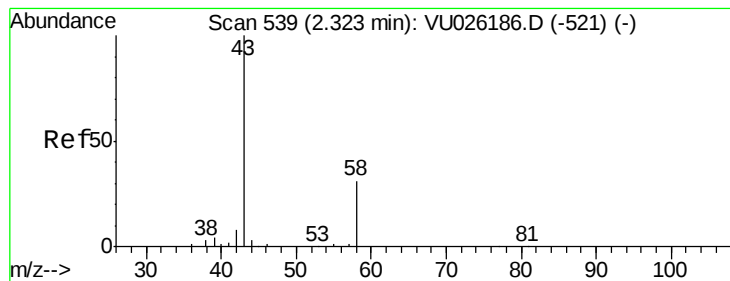

#13

Acetone

Concen: 2.60 ug/L

RT: 2.33 min Scan# 541

Delta R.T. 0.01 min

Lab File: VU026195.D

Acq: 17 Aug 2018 21:49

Instrument :
MSVOA_U
ClientSampleId :
C0363

Tot Ion: 43 Resp: 3117

Ion Ratio Lower Upper

43 100

58 27.9 0.0 59.0

