


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081718\
 Data File : VU026179.D
 Acq On : 17 Aug 2018 15:12
 Operator : MD/SY
 Sample : BFB40
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Aug 18 01:29:07 2018

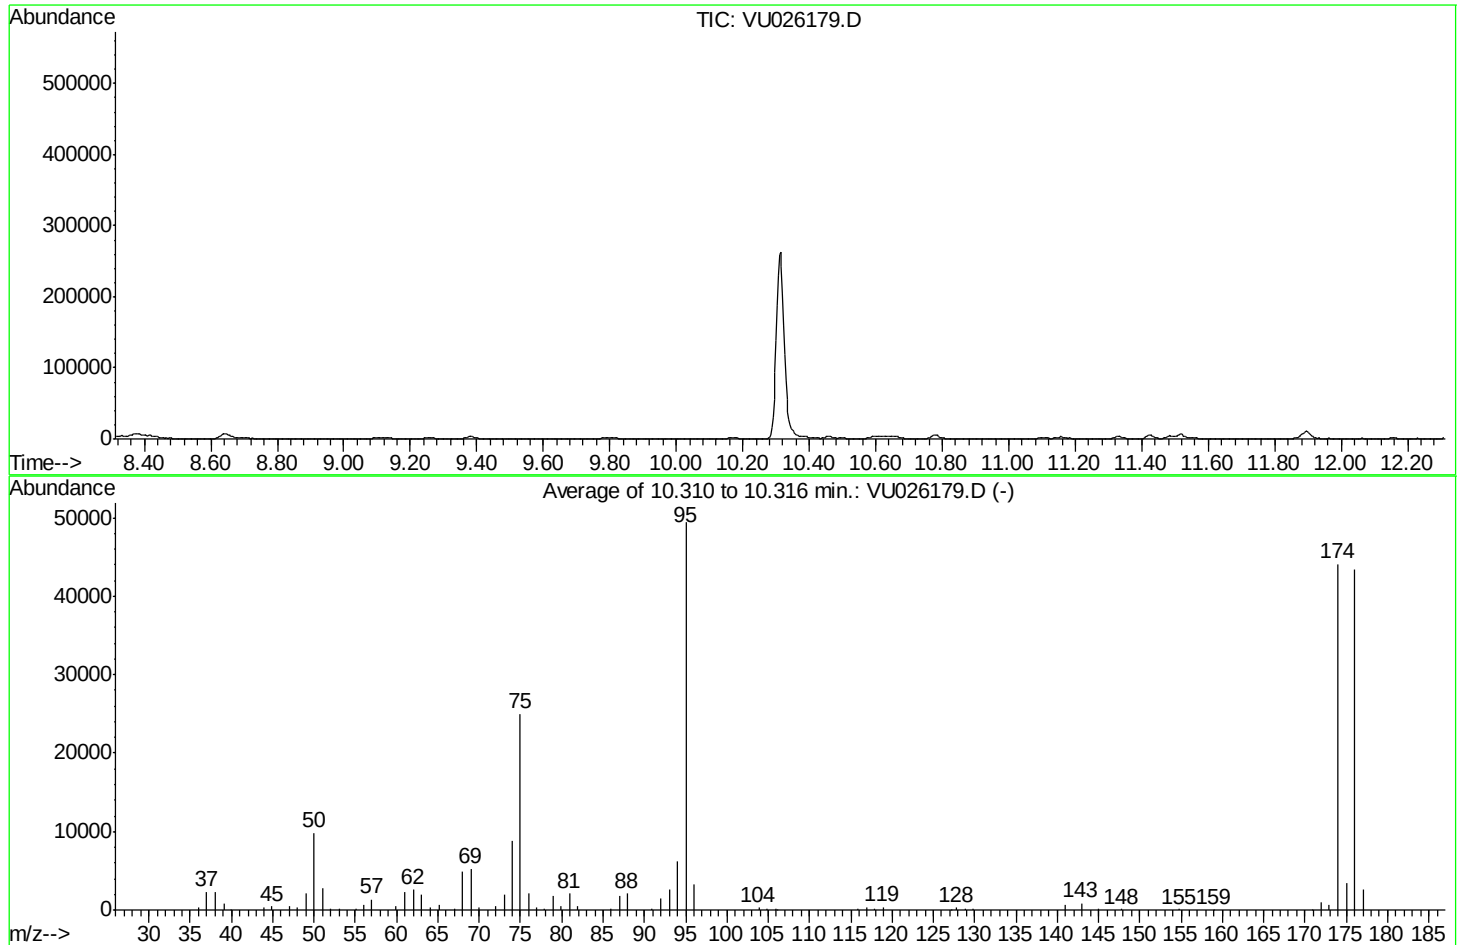

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	9879	PASS
75	95	30	80	50.6	25008	PASS
95	95	100	100	100.0	49432	PASS
96	95	5	9	6.7	3308	PASS
173	174	0.00	2	1.6	711	PASS
174	95	50	120	89.3	44133	PASS
175	174	5	9	7.7	3410	PASS
176	174	95	101	98.3	43389	PASS
177	176	5	9	6.0	2589	PASS

Scan 3010 (10.268 min): VU026179.D
BFB40

m/z	Abundance
39.90	134.0
44.00	528.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	413.0
37.00	2437.0
38.00	2260.0
39.00	749.0
40.00	152.0
44.00	780.0
44.90	465.0
47.00	524.0
48.00	329.0
49.00	2184.0
50.00	10352.0
51.00	2809.0
52.00	143.0
53.00	145.0
55.10	149.0
56.00	752.0
57.00	1307.0
59.90	465.0
61.00	2552.0
62.00	2597.0
63.00	2099.0
64.00	399.0
65.10	655.0
67.00	123.0
68.00	5190.0
69.00	5466.0
69.90	380.0
72.00	422.0
73.10	2120.0
74.00	9072.0
75.00	26208.0
76.00	2026.0
77.00	379.0
77.90	194.0
78.90	1768.0
79.90	553.0
80.90	2065.0
81.90	474.0
86.00	105.0
86.90	2040.0
87.90	2170.0
90.90	210.0
92.00	1438.0
93.00	2761.0
94.00	6346.0
95.00	50744.0
96.00	3254.0
103.90	295.0
104.90	135.0
105.90	220.0
115.90	186.0
117.00	337.0
118.00	222.0
118.90	407.0
127.10	107.0
127.80	258.0
128.70	176.0
129.70	196.0
140.90	650.0
142.90	906.0
145.00	149.0
147.80	146.0
172.00	967.0
173.00	729.0
174.00	43792.0
175.00	3214.0
176.00	43072.0
177.00	2612.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	383.0
37.00	2473.0
38.00	2294.0
39.10	841.0
40.00	174.0
44.00	872.0
44.90	473.0
47.00	603.0
48.00	285.0
49.00	2100.0
50.00	10214.0
51.00	2942.0
52.00	153.0
53.10	135.0
55.10	166.0
56.00	773.0
57.00	1392.0
60.00	489.0
61.00	2394.0
62.00	2706.0
63.00	2086.0
64.00	319.0
65.10	743.0
66.90	185.0
68.00	5018.0
69.00	5491.0
69.90	378.0
72.00	470.0
73.10	2087.0
74.00	8906.0
75.00	25824.0
76.00	2149.0
77.00	391.0
77.90	204.0
78.90	1797.0
80.00	553.0
80.90	2169.0
81.90	500.0
86.00	105.0
87.00	1850.0
87.90	2181.0
90.90	237.0
92.00	1471.0
93.00	2617.0
94.00	6402.0
95.00	51000.0
96.00	3464.0
103.90	332.0
104.90	155.0
105.90	209.0
115.90	231.0
116.90	367.0
117.80	211.0
118.90	417.0
127.80	278.0
128.80	179.0
129.70	173.0
140.90	589.0
142.90	852.0
145.00	152.0
147.80	109.0
154.80	118.0
159.00	105.0
170.90	107.0
172.00	1009.0
173.00	717.0
174.00	45576.0
175.00	3533.0
176.00	45064.0
177.00	2600.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	357.0
37.00	2179.0
38.00	2206.0
39.10	865.0
40.00	170.0
44.00	823.0
44.90	436.0
47.00	582.0
47.90	273.0
49.00	1918.0
50.00	9073.0
51.00	2801.0
52.10	137.0
53.10	100.0
55.00	146.0
56.00	688.0
57.00	1247.0
60.00	420.0
61.00	2122.0
62.00	2348.0
63.00	1921.0
64.00	270.0
65.10	682.0
66.90	226.0
68.00	4424.0
69.00	4951.0
69.90	329.0
72.00	414.0
73.00	1928.0
74.00	8481.0
75.00	22992.0
76.00	2001.0
77.00	341.0
77.90	195.0
78.90	1705.0
80.00	425.0
80.90	1981.0
81.90	519.0
86.00	105.0
87.00	1565.0
87.90	1903.0
91.00	214.0
92.00	1323.0
93.00	2245.0
94.00	5821.0
95.00	46552.0
96.00	3206.0
103.90	294.0
104.90	128.0
106.10	217.0
115.80	201.0
116.90	390.0
117.70	210.0
118.90	346.0
127.80	241.0
128.90	170.0
129.80	154.0
140.90	537.0
142.90	746.0
144.90	186.0
147.90	108.0
154.80	174.0
159.00	123.0
172.00	955.0
172.90	687.0
174.00	43032.0
175.00	3484.0
176.00	42032.0
177.00	2555.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40