


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081720\
 Data File : VU039876.D
 Acq On : 17 Aug 2020 09:13
 Operator : SY/MD
 Sample : BFB15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Aug 18 07:51:41 2020

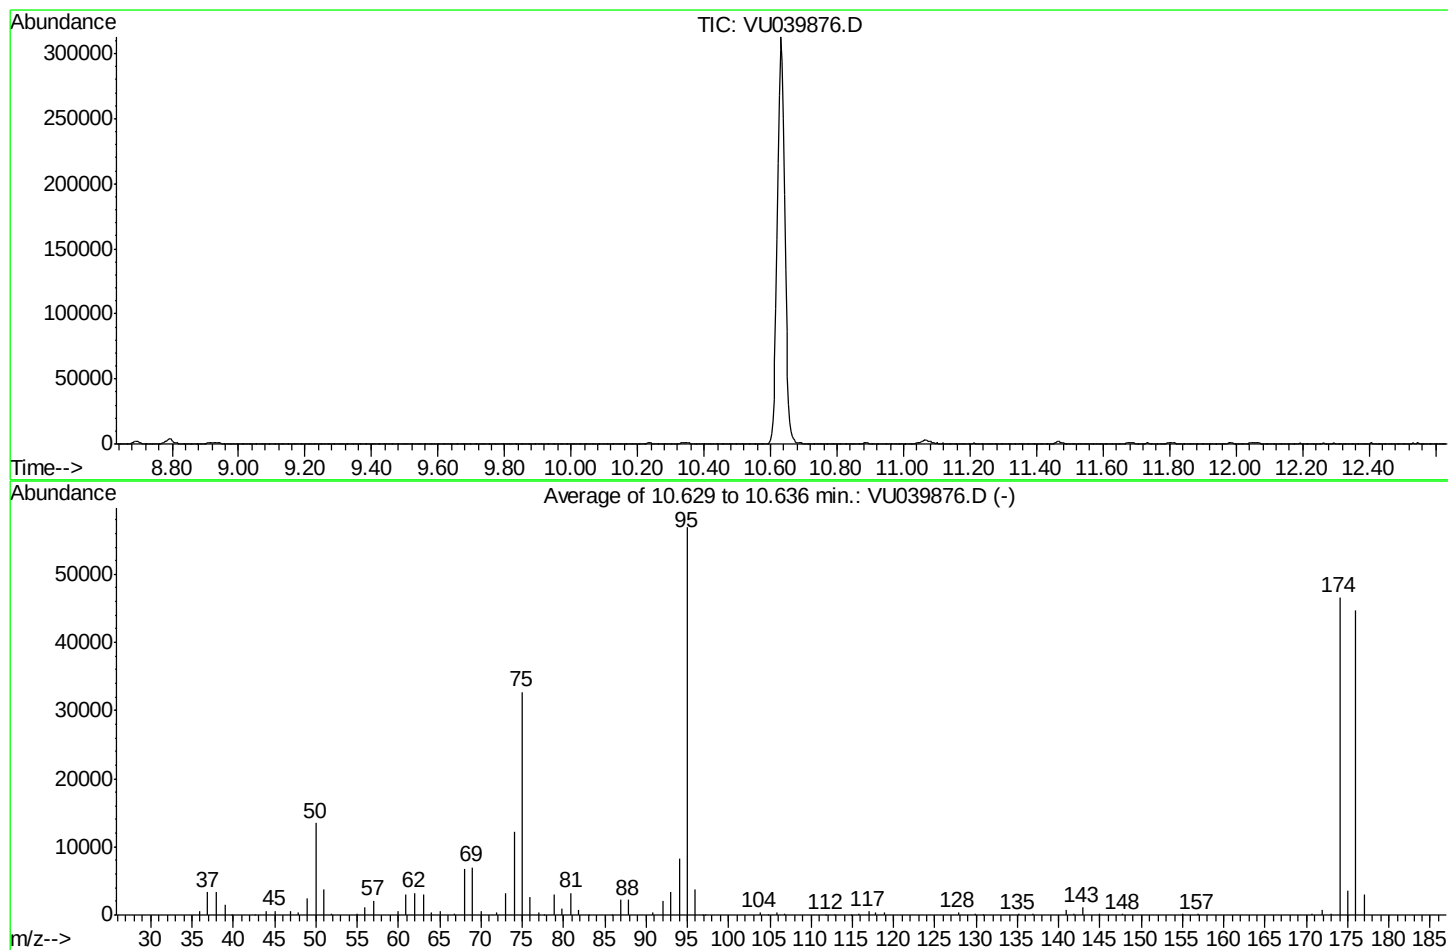

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	13468	PASS
75	95	30	80	57.5	32717	PASS
95	95	100	100	100.0	56880	PASS
96	95	5	9	6.5	3720	PASS
173	174	0.00	2	0.5	211	PASS
174	95	50	120	81.8	46546	PASS
175	174	5	9	7.7	3603	PASS
176	174	95	101	96.2	44776	PASS
177	176	5	9	6.7	2981	PASS

m/z	Abundance
35.90	521.0
36.90	3209.0
37.90	3412.0
39.00	1518.0
44.00	696.0
45.00	578.0
47.00	583.0
47.80	284.0
48.90	2530.0
50.00	13114.0
51.00	3838.0
51.80	209.0
55.00	159.0
55.90	1192.0
56.90	2214.0
60.00	578.0
61.00	3089.0
62.00	3266.0
63.00	2996.0
64.00	300.0
65.00	652.0
66.90	211.0
68.00	6829.0
68.90	7090.0
70.00	524.0
71.90	310.0
73.00	3316.0
74.00	12481.0
75.00	32808.0
76.00	2751.0
77.00	385.0
78.90	3062.0
79.80	1039.0
80.90	3297.0
81.80	888.0
83.00	120.0
85.90	117.0
86.90	2212.0
87.80	2224.0
90.80	464.0
92.00	1926.0
93.00	3130.0
94.00	8447.0
95.00	57032.0
96.00	3600.0
96.90	143.0
103.80	272.0
104.80	118.0
105.90	343.0
106.70	187.0
114.90	100.0
115.80	315.0
117.00	521.0
117.80	391.0
118.90	424.0
127.80	310.0
129.90	199.0
135.10	103.0
136.90	135.0
140.90	717.0
141.80	146.0
142.90	982.0
144.90	157.0
147.70	100.0
156.80	181.0
170.60	120.0
171.90	727.0
174.00	45800.0
175.00	3620.0
176.00	44384.0
176.90	2911.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
35.80	480.0
36.90	3486.0
37.90	3343.0
39.00	1634.0
42.70	123.0
44.00	766.0
45.00	619.0
47.00	574.0
47.90	319.0
49.00	2427.0
50.00	13896.0
51.00	3873.0
51.90	280.0
55.00	182.0
55.90	1305.0
56.90	2140.0
60.00	597.0
61.00	3071.0
61.90	3366.0
63.00	3145.0
64.10	322.0
65.00	574.0
66.80	191.0
68.00	6990.0
69.00	7324.0
70.00	551.0
71.80	345.0
73.00	3340.0
74.00	12500.0
75.00	33824.0
76.00	2665.0
77.00	299.0
78.90	3109.0
79.90	1023.0
80.90	3435.0
81.90	842.0
86.90	2234.0
87.80	2203.0
90.90	389.0
92.00	2107.0
93.00	3547.0
94.00	8421.0
95.00	58784.0
96.00	3829.0
97.10	148.0
103.80	311.0
105.90	336.0
106.80	142.0
112.90	108.0
114.90	112.0
115.80	297.0
117.00	500.0
117.80	392.0
118.90	454.0
127.80	394.0
129.90	271.0
130.80	117.0
135.10	152.0
136.80	140.0
140.90	779.0
141.90	128.0
142.90	1136.0
144.90	171.0
147.70	135.0
155.00	155.0
156.80	159.0
170.60	130.0
172.00	743.0
174.00	47968.0
175.00	3745.0
176.00	46096.0
177.00	3108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	435.0
36.90	3252.0
38.00	3141.0
39.00	1484.0
39.80	132.0
42.60	122.0
44.00	779.0
45.00	572.0
47.00	507.0
48.00	338.0
49.00	2320.0
50.00	13395.0
51.00	3671.0
51.90	272.0
55.00	194.0
55.90	1175.0
57.00	1983.0
60.00	591.0
60.90	2786.0
61.90	3165.0
63.00	2917.0
64.10	306.0
65.00	455.0
66.70	182.0
68.00	6560.0
69.00	6598.0
70.00	560.0
71.90	317.0
73.00	2895.0
74.00	11394.0
75.00	31520.0
76.00	2381.0
76.90	264.0
77.70	282.0
78.90	2928.0
79.90	945.0
80.90	3058.0
81.90	712.0
86.90	2071.0
87.90	2156.0
90.80	272.0
92.00	2015.0
93.00	3478.0
94.00	7687.0
95.00	54824.0
96.00	3731.0
97.10	148.0
103.80	406.0
105.90	288.0
111.80	103.0
115.90	243.0
117.00	465.0
117.80	321.0
119.00	456.0
127.80	374.0
129.90	320.0
130.80	122.0
135.10	158.0
136.80	107.0
140.90	742.0
141.90	116.0
142.90	1070.0
144.90	159.0
147.80	144.0
154.90	183.0
156.80	117.0
170.60	111.0
172.00	748.0
173.00	633.0
174.00	45872.0
175.00	3446.0
176.00	43848.0
177.00	2925.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
43.90	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15