

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081721\
 Data File : VU044438.D
 Acq On : 17 Aug 2021 13:57
 Operator : SY/MD
 Sample : VU0817WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK002

Quant Time: Aug 18 01:41:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 17 02:56:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	5888	0.500	ug/L	0.02
5) Chlorobenzene-d5	9.361	117	5591	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.759	152	2907	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	3672	0.477	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	96.000%		
4) 1,2-Dichloroethane-d4	5.679	65	4032	0.456	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
7) 1,2-Dichloropropane-d6	6.639	67	3311	0.482	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	96.000%		
8) Toluene-d8	7.845	98	7514	0.478	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
10) 1,1,2,2-Tetrachloroeth...	10.696	84	2812	0.482	ug/L	0.02
Spiked Amount 0.500	Range 65 - 120		Recovery =	96.000%		
Target Compounds					Qvalue	
13) 1,2-Dibromo-3-chloropr...	13.147	75	25	0.031	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081721\
Data File : VU044438.D
Acq On : 17 Aug 2021 13:57
Operator : SY/MD
Sample : VU0817WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002


Quant Time: Aug 18 01:41:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 17 02:56:51 2021
Response via : Initial Calibration

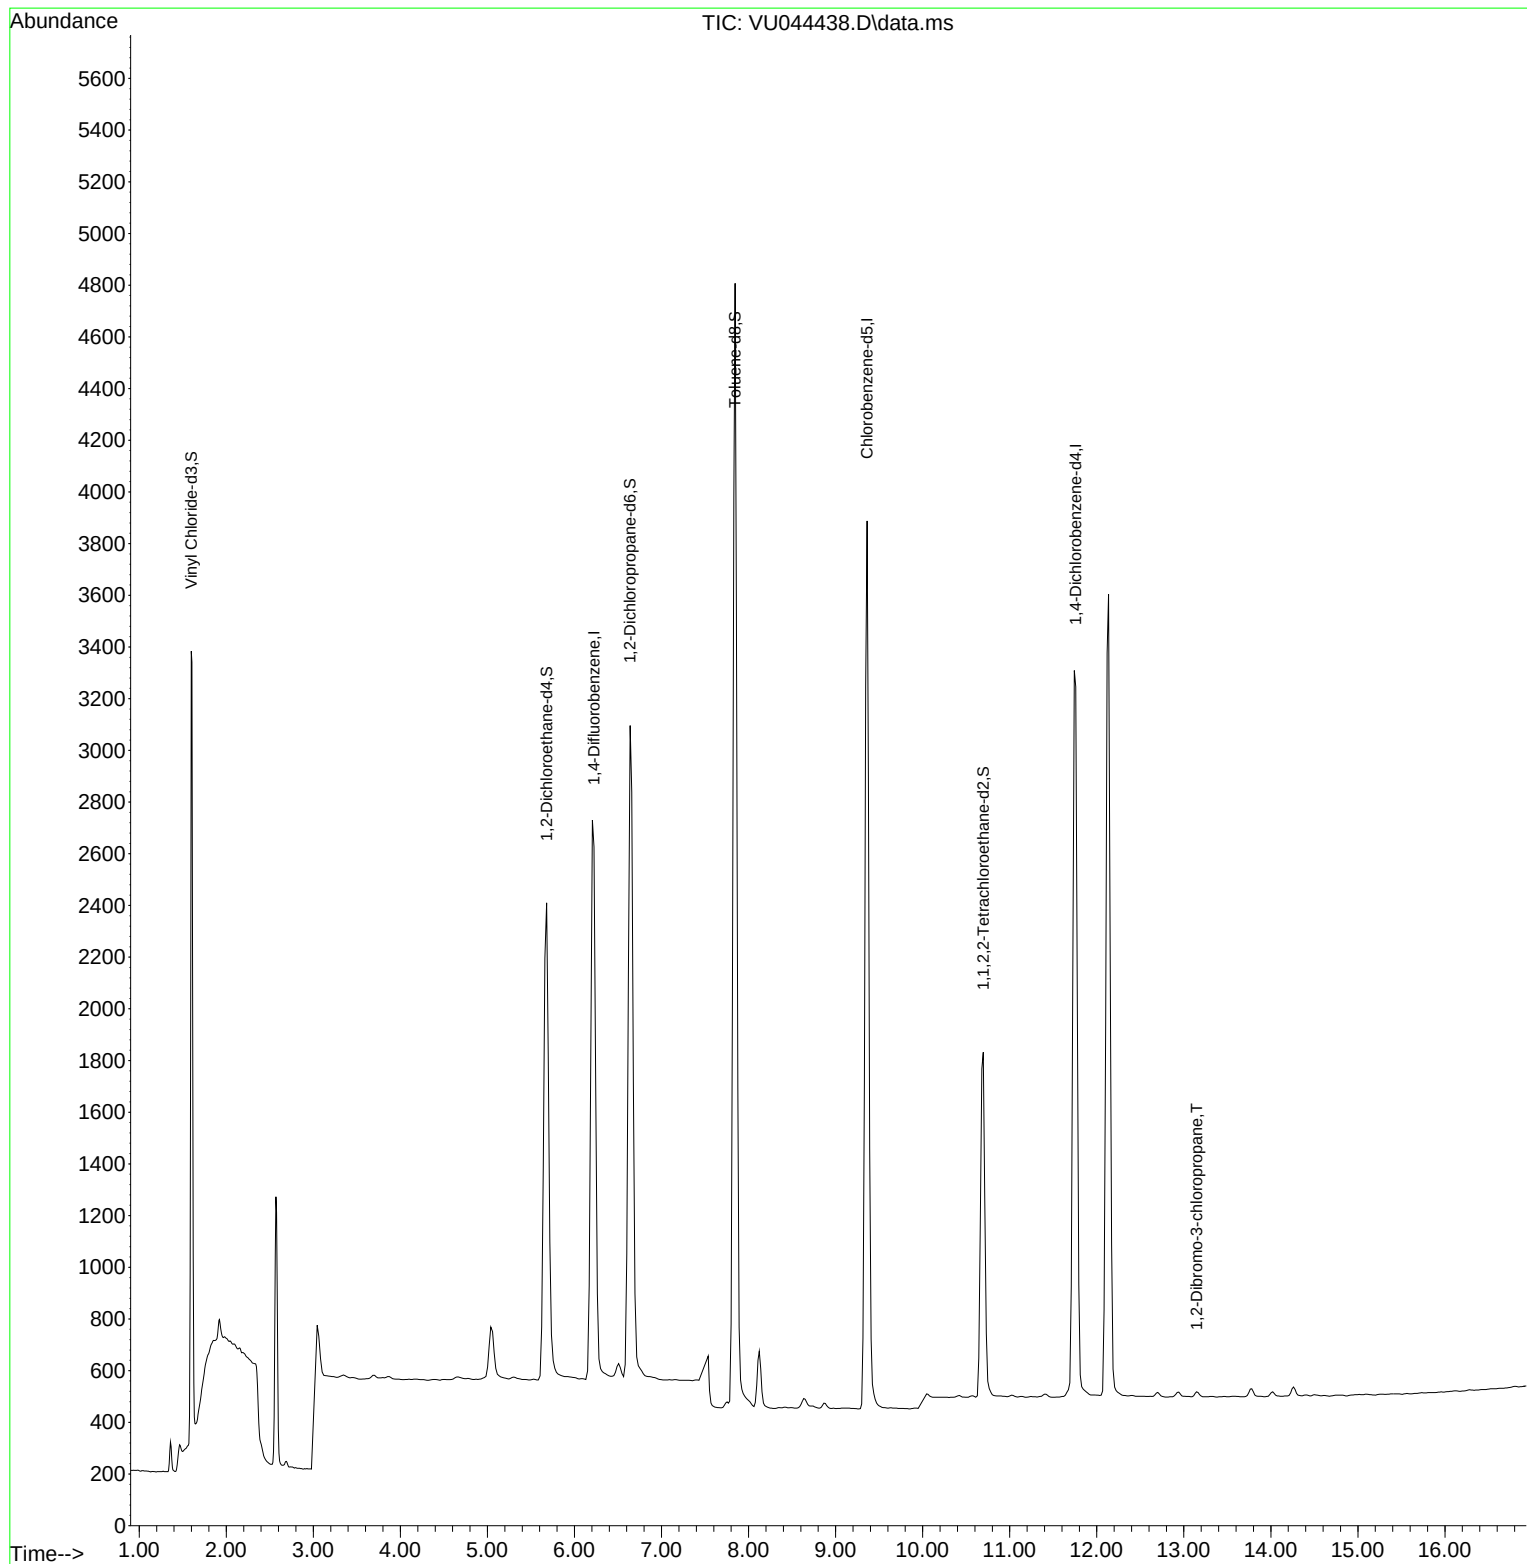

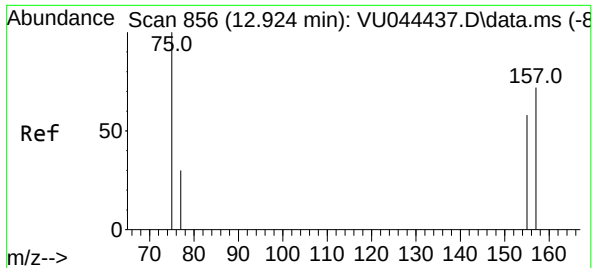

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.031 ug/L
 RT: 13.147 min Scan# 869
 Delta R.T. 0.223 min
 Lab File: VU044438.D
 Acq: 17 Aug 2021 13:57

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK002

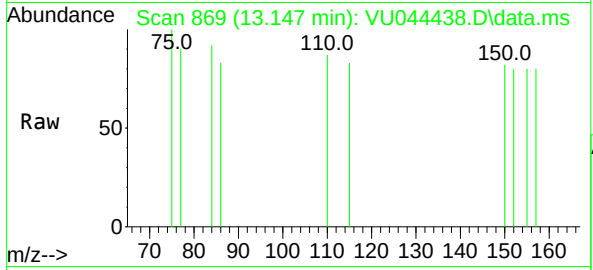

Tgt Ion: 75	Resp:	25
Ion	Ratio	Lower Upper
75	100	
157	80.0	63.5 95.3
155	80.0	56.2 84.4

