


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081721\
Data File : VU044436.D
Acq On : 17 Aug 2021 09:24
Operator : SY/MD
Sample : BFB003
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB003

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081621.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 17 02:56:51 2021

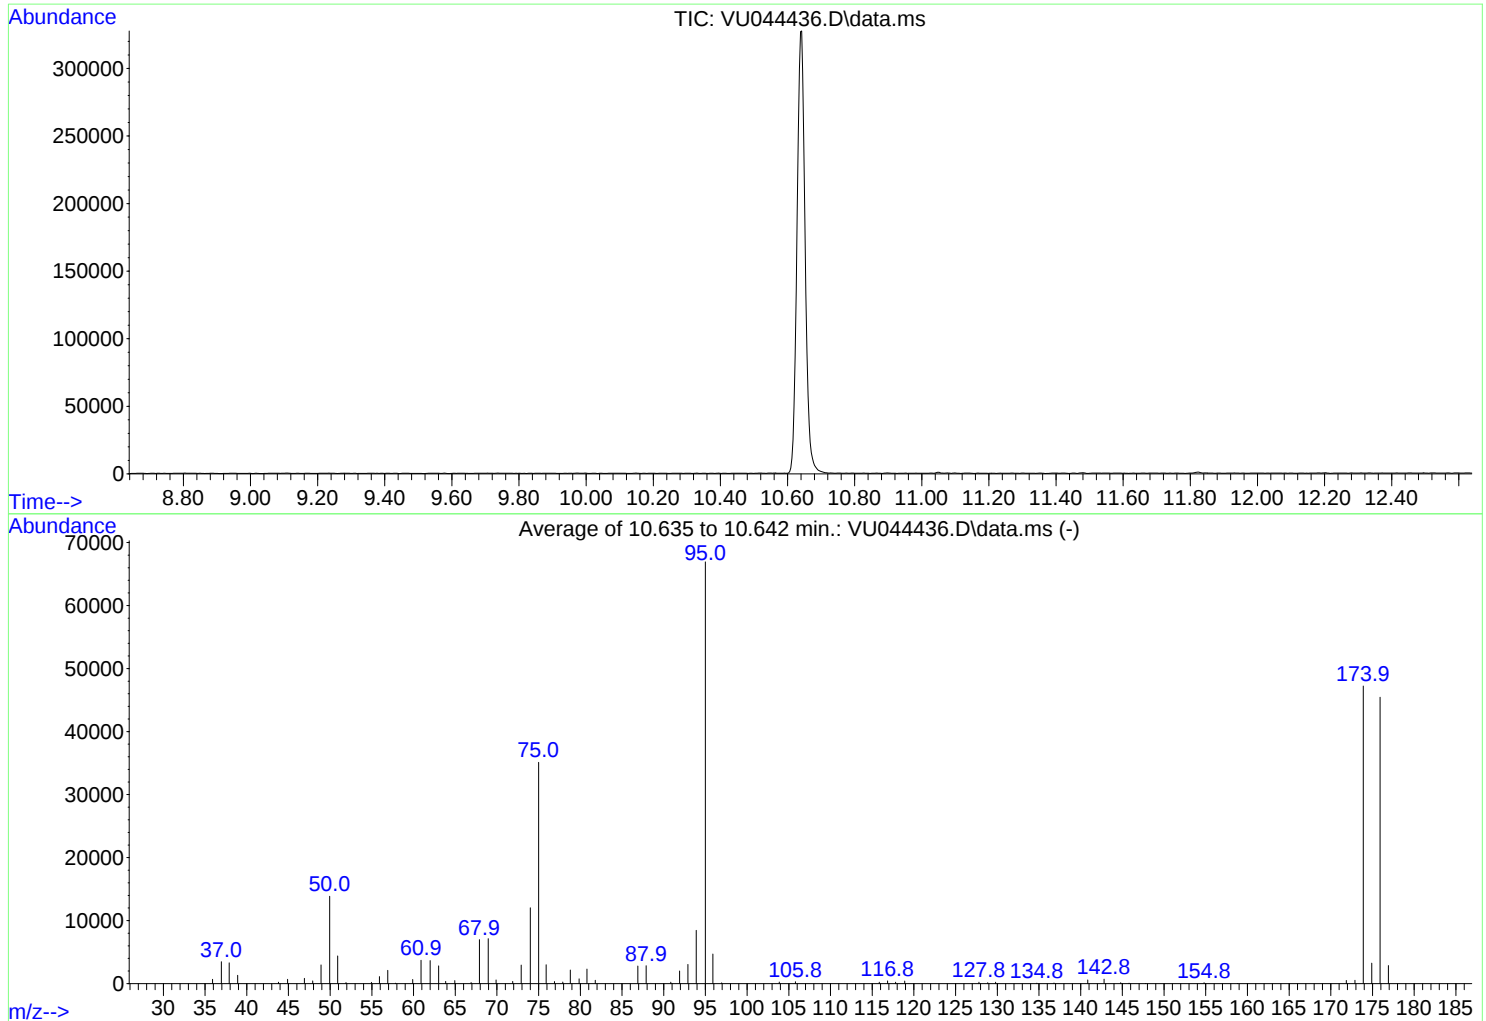

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	13856	PASS
75	95	30	80	52.5	35131	PASS
95	95	100	100	100.0	66936	PASS
96	95	5	9	7.0	4692	PASS
173	174	0.00	2	1.1	540	PASS
174	95	50	120	70.6	47235	PASS
175	174	5	9	6.9	3257	PASS
176	174	95	101	96.2	45443	PASS
177	176	5	9	6.3	2873	PASS