


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081819\
 Data File : VU033828.D
 Acq On : 16 Aug 2019 11:59
 Operator : JC/SP
 Sample : BFB58
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB58

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 19 13:39:42 2019

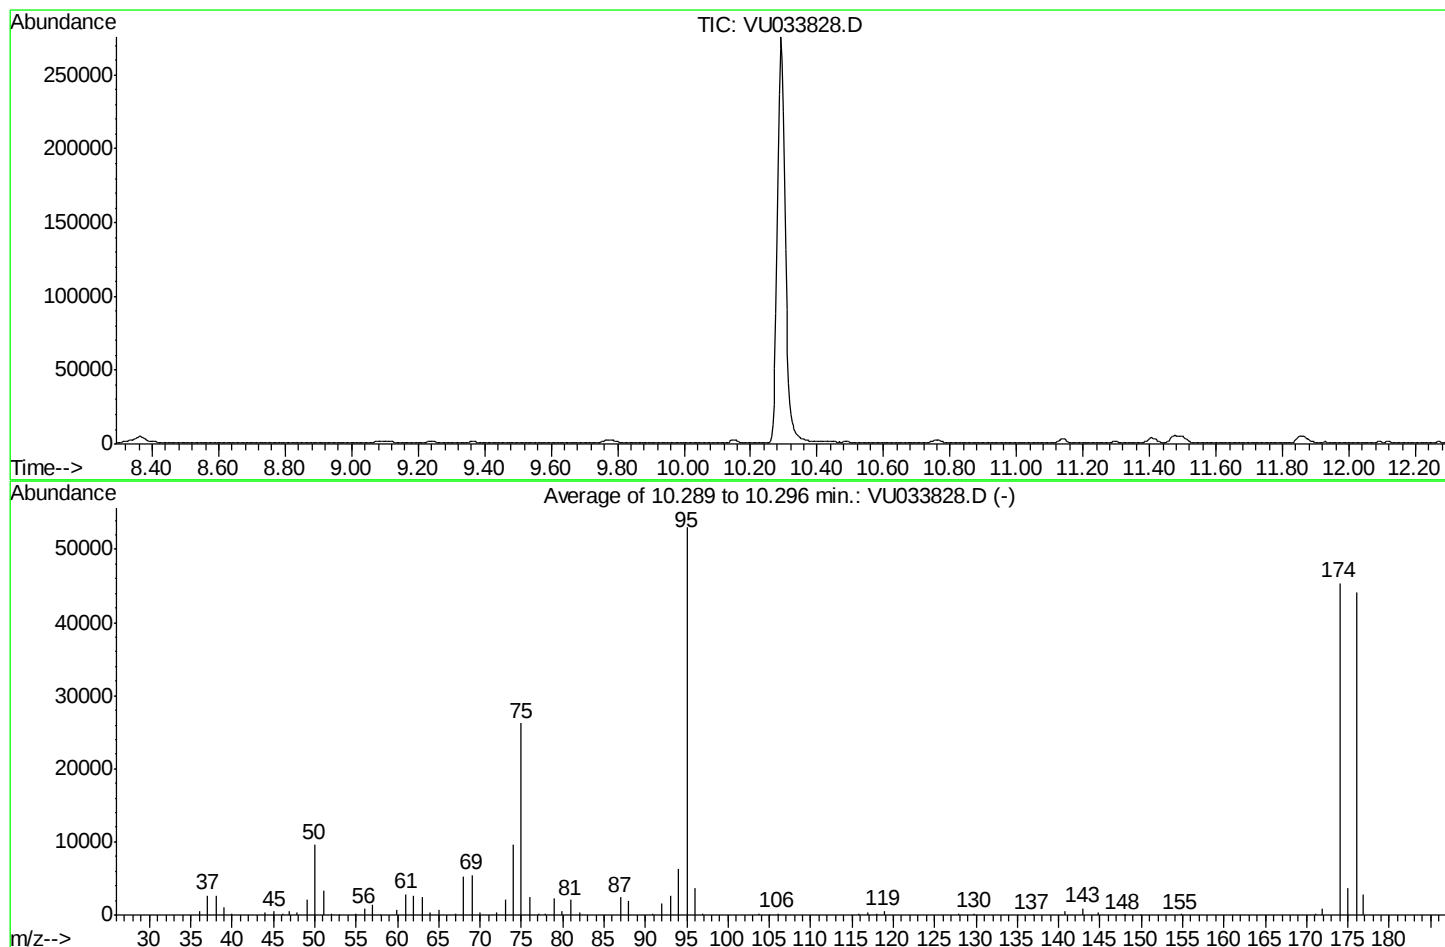

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	9591	PASS
75	95	30	80	49.5	26232	PASS
95	95	100	100	100.0	53024	PASS
96	95	5	9	6.9	3638	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.5	45354	PASS
175	174	5	9	8.0	3627	PASS
176	174	95	101	97.4	44194	PASS
177	176	5	9	6.3	2801	PASS

m/z	Abundance
36.00	464.0
37.00	2684.0
38.00	2516.0
39.00	1125.0
40.00	319.0
43.90	898.0
45.10	468.0
46.10	174.0
46.90	564.0
47.90	335.0
49.00	2167.0
50.00	9860.0
51.10	3334.0
52.10	145.0
53.00	144.0
55.00	126.0
56.00	822.0
57.00	1389.0
59.90	724.0
61.00	2889.0
62.00	2672.0
63.00	2485.0
64.00	400.0
65.00	675.0
67.00	172.0
68.00	5276.0
69.00	5343.0
70.00	364.0
71.90	263.0
73.00	2061.0
74.00	10081.0
75.00	26792.0
76.00	2703.0
77.00	253.0
77.90	219.0
78.90	2266.0
79.90	586.0
81.00	2271.0
82.00	372.0
87.00	2402.0
88.00	1987.0
90.80	239.0
92.00	1632.0
93.00	2563.0
94.00	6071.0
95.00	53088.0
96.00	3617.0
96.90	118.0
103.80	225.0
104.90	144.0
106.00	257.0
115.80	289.0
116.80	363.0
118.00	205.0
118.90	623.0
127.90	191.0
129.80	250.0
136.80	121.0
140.80	655.0
142.90	901.0
144.80	278.0
147.80	140.0
149.90	129.0
154.80	117.0
171.20	161.0
172.00	751.0
174.00	44408.0
175.00	3758.0
176.00	42960.0
176.90	2891.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	476.0
37.00	2738.0
38.00	2771.0
39.00	1171.0
40.00	331.0
43.90	842.0
45.00	491.0
46.10	164.0
46.90	524.0
47.90	320.0
49.00	2201.0
50.00	9849.0
51.10	3425.0
52.00	185.0
55.00	143.0
56.00	882.0
57.00	1475.0
60.00	782.0
61.00	2949.0
62.00	2670.0
63.00	2604.0
64.00	350.0
65.10	681.0
67.00	155.0
68.00	5386.0
69.00	5605.0
70.00	387.0
72.00	270.0
73.00	2175.0
74.00	9952.0
75.00	26880.0
76.00	2542.0
77.10	251.0
77.90	216.0
78.90	2264.0
79.90	565.0
81.00	2103.0
82.00	421.0
87.00	2509.0
87.90	1971.0
90.80	225.0
92.00	1606.0
93.00	2576.0
94.00	6601.0
95.00	54712.0
96.10	3750.0
97.00	151.0
103.70	207.0
104.90	123.0
106.00	239.0
115.80	235.0
116.90	410.0
118.00	188.0
118.90	612.0
127.90	199.0
129.80	262.0
140.80	602.0
142.90	991.0
144.90	299.0
147.80	136.0
150.00	116.0
154.80	127.0
171.10	169.0
171.90	908.0
174.00	46568.0
175.00	3760.0
176.00	45504.0
176.90	2846.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	454.0
37.00	2528.0
38.00	2660.0
39.00	997.0
40.00	328.0
43.90	791.0
45.00	442.0
46.90	335.0
47.90	287.0
49.00	2151.0
50.00	9066.0
51.00	3136.0
51.90	195.0
54.90	148.0
56.00	812.0
57.00	1436.0
57.90	142.0
60.00	660.0
61.00	2692.0
62.00	2480.0
63.00	2413.0
64.00	315.0
65.10	656.0
67.10	148.0
68.00	5208.0
69.00	5339.0
70.10	326.0
72.00	296.0
73.00	2133.0
74.00	8902.0
75.00	25024.0
76.00	2161.0
77.00	253.0
77.90	241.0
78.90	2145.0
80.00	476.0
80.90	1854.0
82.00	368.0
87.00	2244.0
87.90	1844.0
90.90	194.0
92.00	1489.0
93.00	2518.0
94.00	6509.0
95.00	51272.0
96.10	3549.0
97.00	158.0
103.90	181.0
106.00	204.0
115.90	191.0
117.00	417.0
117.80	123.0
118.10	141.0
118.90	502.0
127.80	157.0
129.80	244.0
140.80	508.0
143.00	895.0
144.90	340.0
148.00	135.0
154.80	109.0
171.10	177.0
171.90	1060.0
174.00	45088.0
175.00	3365.0
176.00	44120.0
176.90	2667.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

Scan 2849 (10.251 min): VU033828.D
BFB58

m/z	Abundance
39.80	174.0
43.90	450.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58