


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081821\
Data File : VU044455.D
Acq On : 18 Aug 2021 19:24
Operator : SY/MD
Sample : M3474-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

MMDadoda
8/19/2021 3:31:43 PM

Quant Time: Aug 19 04:05:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 19 03:54:51 2021
Response via : Initial Calibration

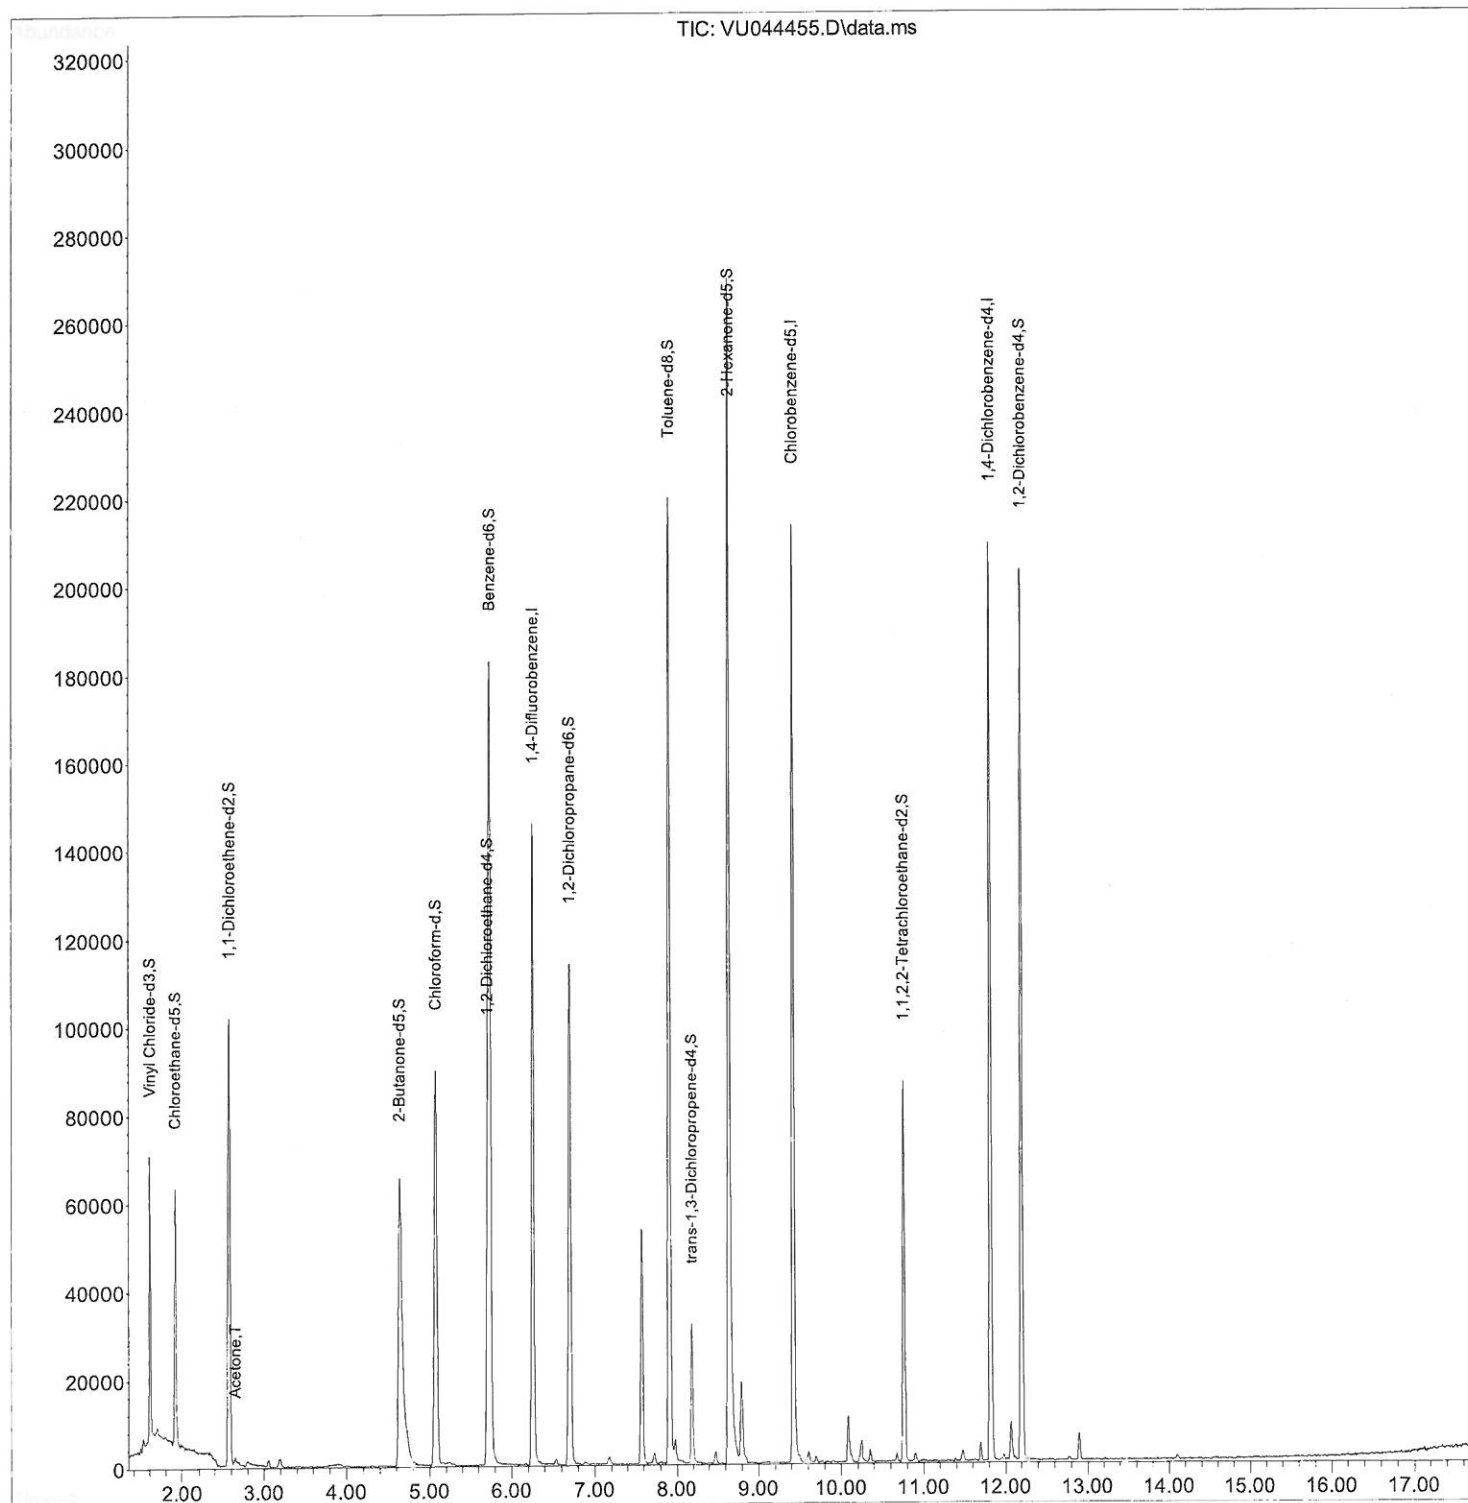

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081821\
 Data File : VU044455.D
 Acq On : 18 Aug 2021 19:24
 Operator : SY/MD
 Sample : M3474-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:31:43 PM

Quant Time: Aug 19 04:05:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 19 03:54:51 2021
 Response via : Initial Calibration

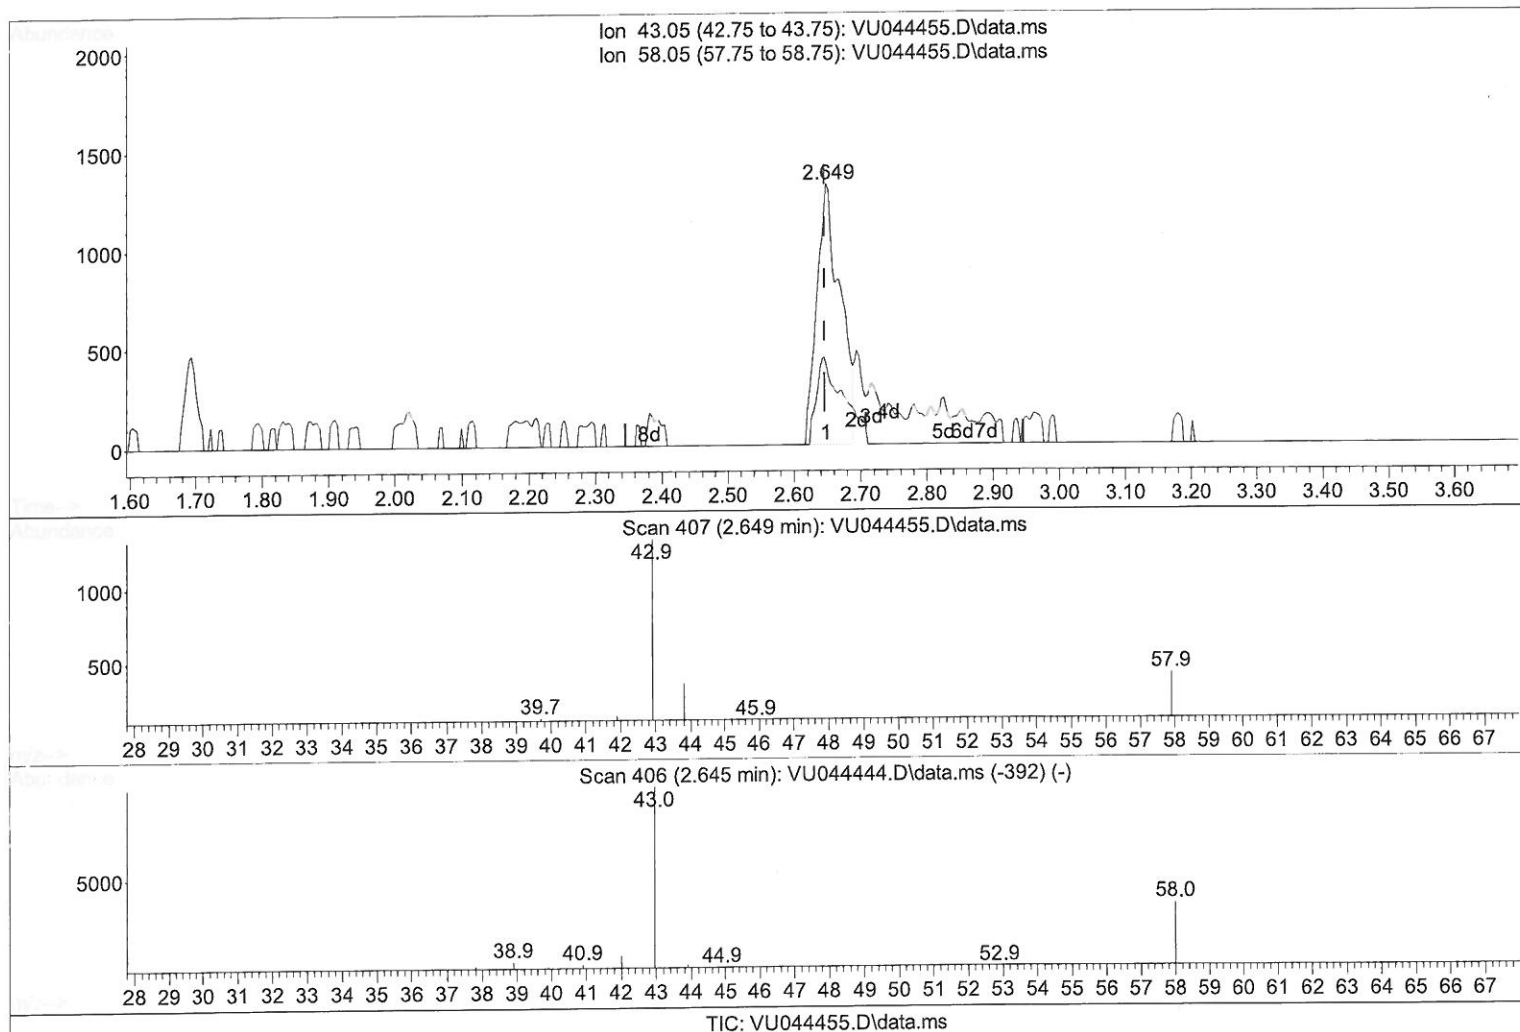

(13) Acetone (T)

2.649min (+ 0.003) 1.49 ug/L

response 3206

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	22.70	23.86
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081821\
 Data File : VU044455.D
 Acq On : 18 Aug 2021 19:24
 Operator : SY/MD
 Sample : M3474-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:31:43 PM

Quant Time: Aug 19 04:05:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 19 03:54:51 2021
 Response via : Initial Calibration

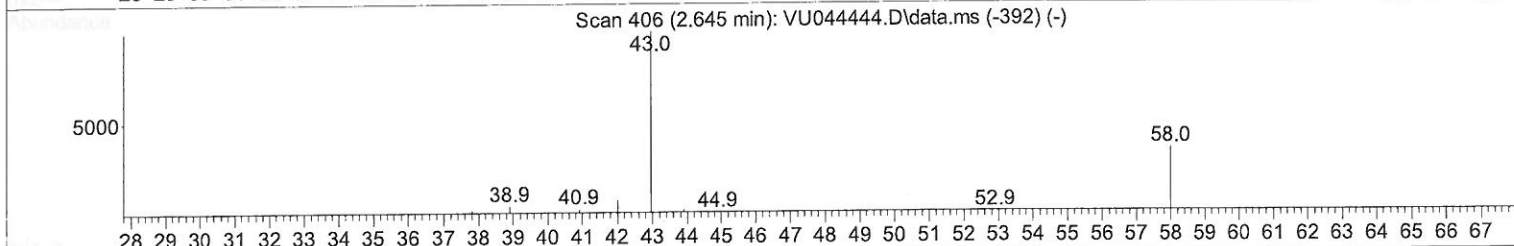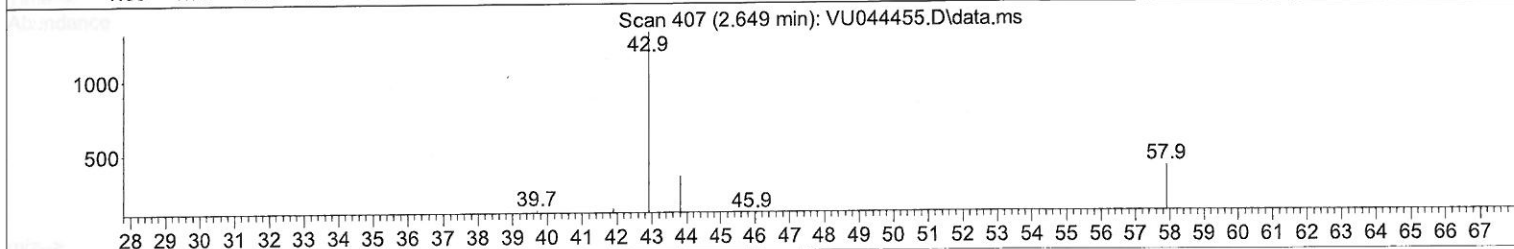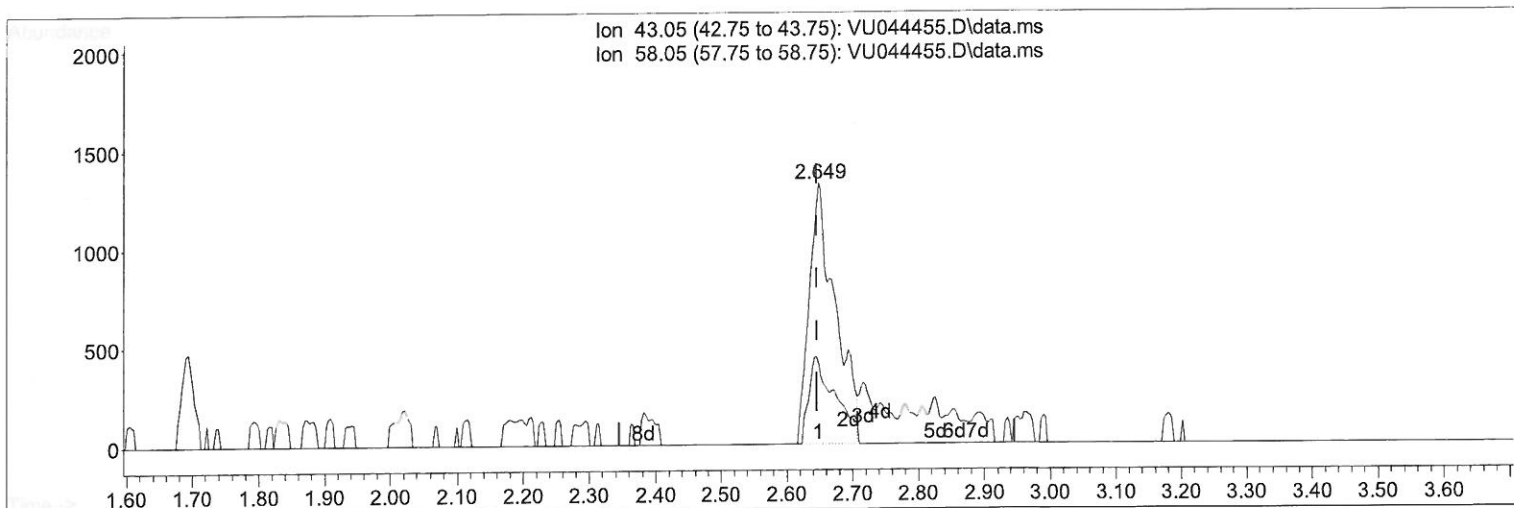

TIC: VU044455.D\data.ms

(13) Acetone (T)

2.649min (+ 0.003) 1.69 ug/L m

response 3633

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	22.70	21.06
0.00	0.00	0.00
0.00	0.00	0.00

2 MD
 8/20/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081821\
 Data File : VU044455.D
 Acq On : 18 Aug 2021 19:24
 Operator : SY/MD
 Sample : M3474-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:31:43 PM

Quant Time: Aug 19 04:05:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 19 03:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	115796	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	116769	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	51904	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	45349	4.842	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 96.800%			
7) Chloroethane-d5	1.916	69	41711	5.125	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 102.400%			
11) 1,1-Dichloroethene-d2	2.571	65	19443	4.880	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 97.600%			
20) 2-Butanone-d5	4.639	46	136796	52.816	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 105.640%			
24) Chloroform-d	5.070	84	82179	4.962	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 99.200%			
26) 1,2-Dichloroethane-d4	5.710	65	48029	5.318	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 106.400%			
32) Benzene-d6	5.735	84	169472	5.154	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 103.000%			
36) 1,2-Dichloropropane-d6	6.700	67	54525	5.183	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 103.600%			
41) Toluene-d8	7.906	98	143977	4.938	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 98.800%			
43) trans-1,3-Dichloroprop...	8.185	79	17876	4.732	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 94.600%			
46) 2-Hexanone-d5	8.645	63	108813	53.264	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 106.520%			
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44319	5.003	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 100.000%			
66) 1,2-Dichlorobenzene-d4	12.198	152	49003	5.588	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 111.800%			
Target Compounds						
13) Acetone	2.649	43	3633m	1.689	ug/L	Qvalue

MD
 8/20/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed