

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081821\
 Data File : VU044455.D
 Acq On : 18 Aug 2021 19:24
 Operator : SY/MD
 Sample : M3474-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:31:43 PM

Quant Time: Aug 19 04:05:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 19 03:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	115796	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	116769	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	51904	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	45349	4.842	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	96.800%	
7) Chloroethane-d5	1.916	69	41711	5.125	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.400%	
11) 1,1-Dichloroethene-d2	2.571	65	19443	4.880	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	97.600%	
20) 2-Butanone-d5	4.639	46	136796	52.816	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.640%	
24) Chloroform-d	5.070	84	82179	4.962	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
26) 1,2-Dichloroethane-d4	5.710	65	48029	5.318	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.400%	
32) Benzene-d6	5.735	84	169472	5.154	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.000%	
36) 1,2-Dichloropropane-d6	6.700	67	54525	5.183	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.600%	
41) Toluene-d8	7.906	98	143977	4.938	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.800%	
43) trans-1,3-Dichloroprop...	8.185	79	17876	4.732	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.645	63	108813	53.264	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	106.520%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44319	5.003	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.000%	
66) 1,2-Dichlorobenzene-d4	12.198	152	49003	5.588	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.800%	
Target Compounds					Qvalue	
13) Acetone	2.649	43	3633m	1.689	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081821\
Data File : VU044455.D
Acq On : 18 Aug 2021 19:24
Operator : SY/MD
Sample : M3474-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

MMDadoda
8/19/2021 3:31:43 PM


Quant Time: Aug 19 04:05:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 19 03:54:51 2021
Response via : Initial Calibration

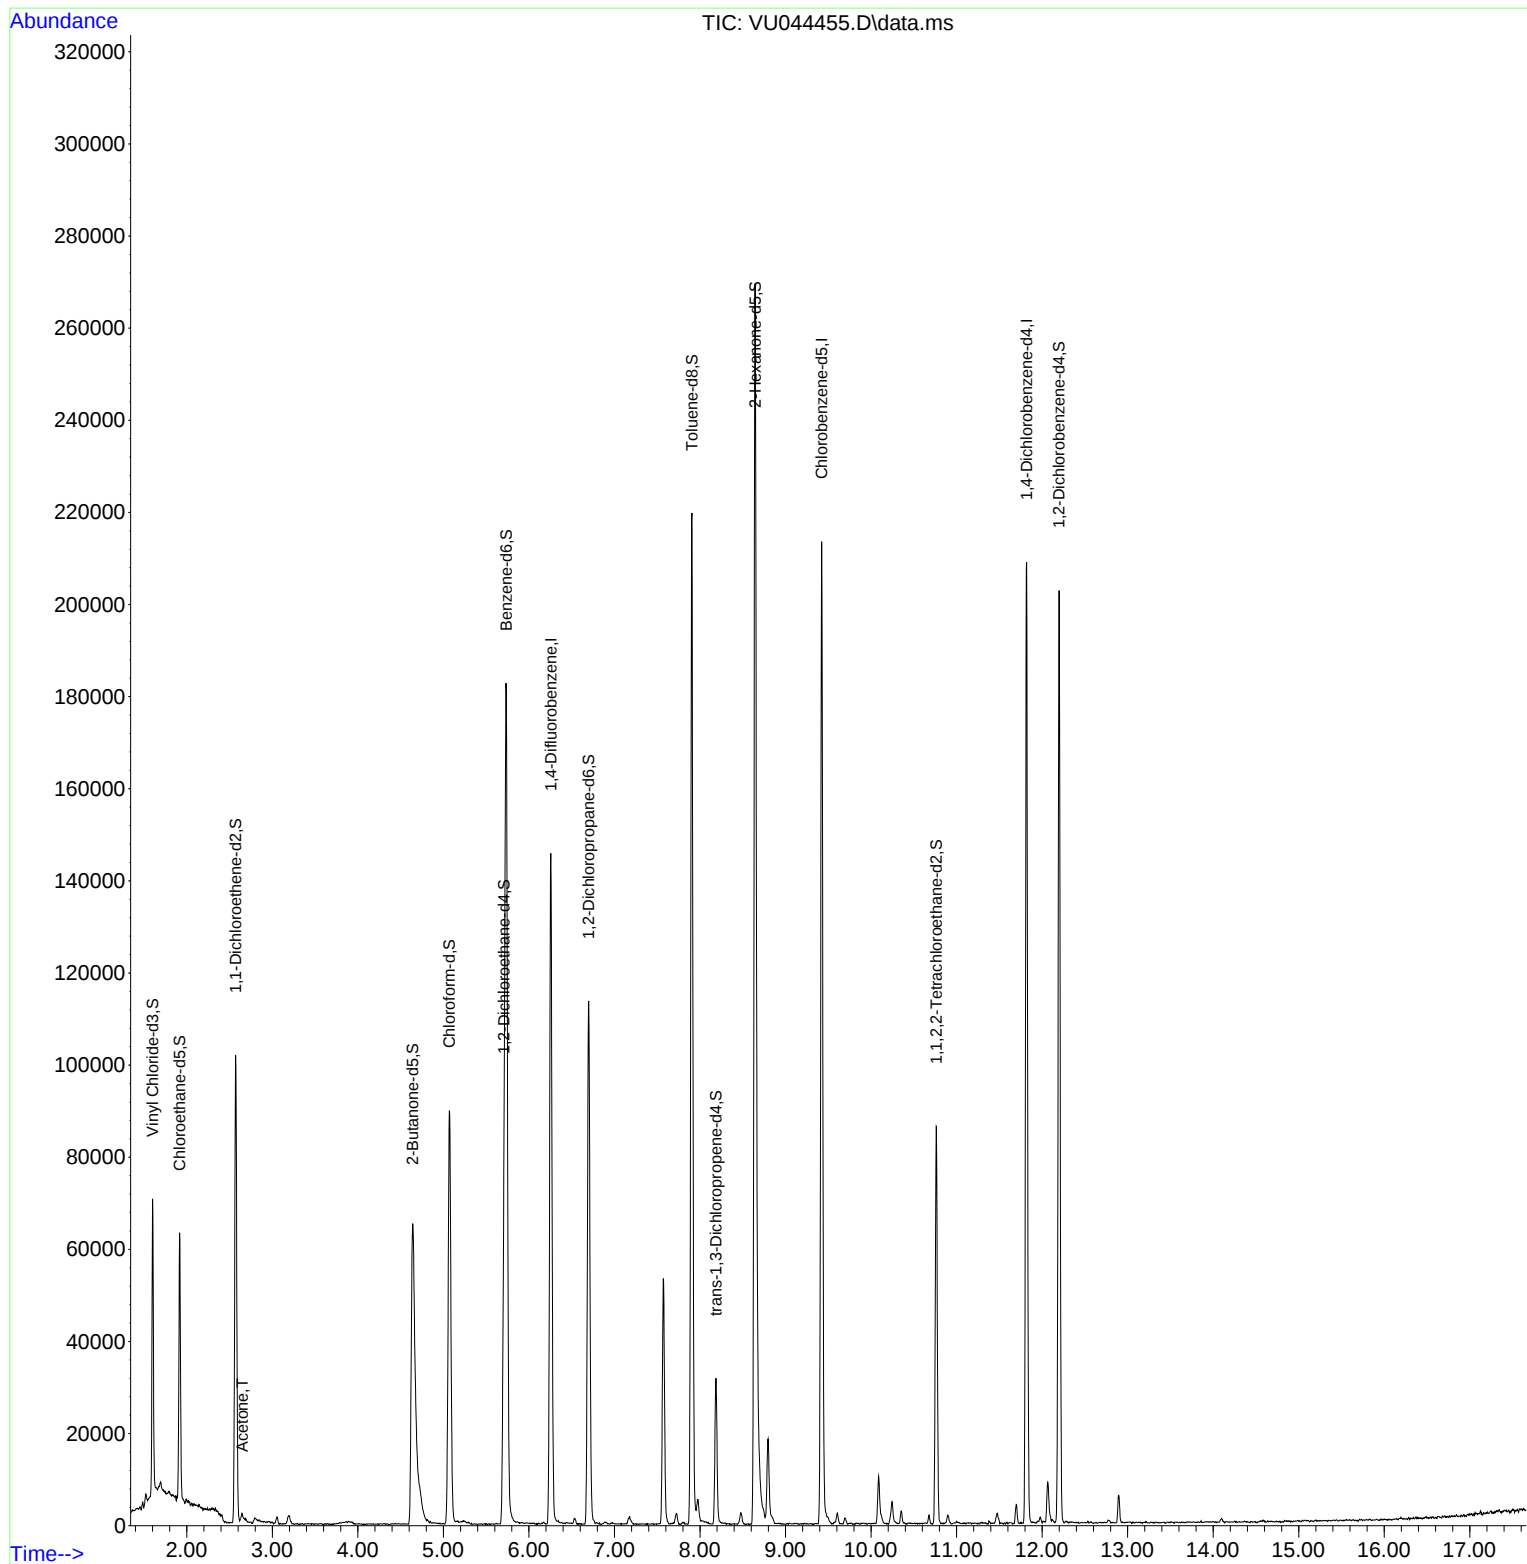

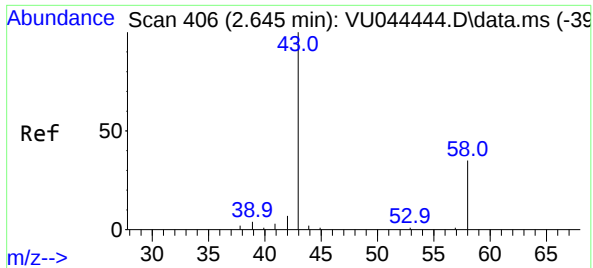

#13
Acetone
Concen: 1.689 ug/L m
RT: 2.649 min Scan# 407
Delta R.T. 0.003 min
Lab File: VU044455.D
Acq: 18 Aug 2021 19:24

Instrument :
MSVOA_U
ClientSampleId :
C0AD3

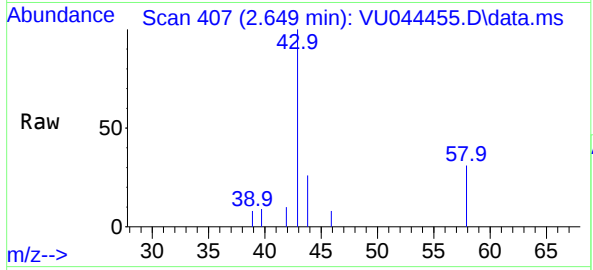

Tgt Ion:	43	Resp:	3633
Ion Ratio	Lower	Upper	
43	100		
58	21.1	0.0	45.4

Manual Integrations
APPROVED
MMDadoda
8/19/2021 3:31:43 PM

