


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081919\
Data File : VU033835.D
Acq On : 19 Aug 2019 08:19
Operator : JC/SP
Sample : BFB03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR081419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 17 01:44:12 2019

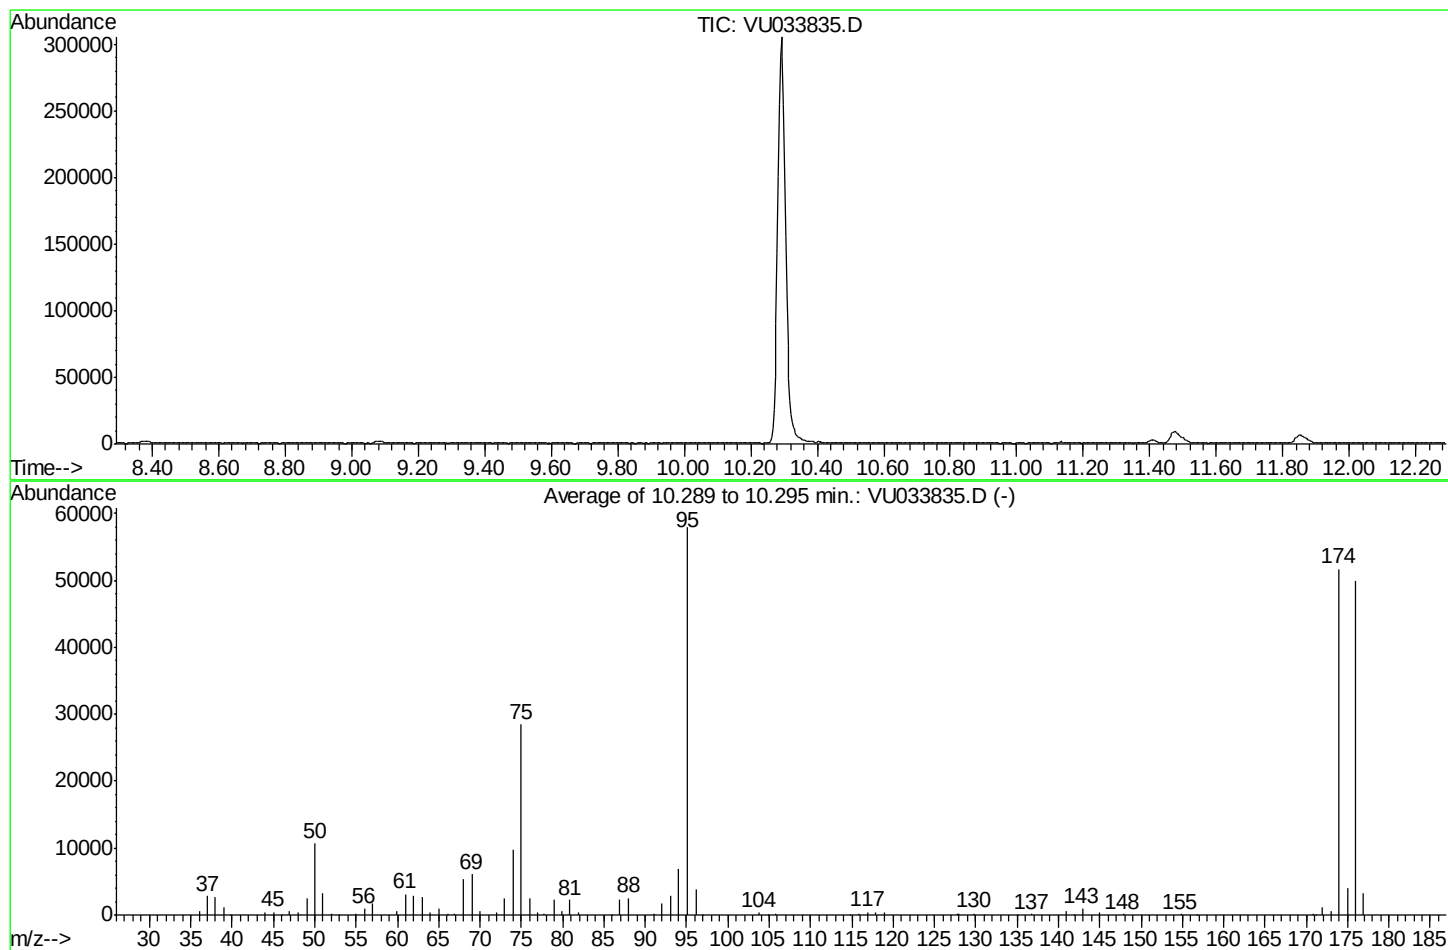

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	10654	PASS
75	95	30	80	49.1	28442	PASS
95	95	100	100	100.0	57933	PASS
96	95	5	9	6.6	3829	PASS
173	174	0.00	2	1.2	637	PASS
174	95	50	120	89.2	51656	PASS
175	174	5	9	7.9	4059	PASS
176	174	95	101	96.6	49906	PASS
177	176	5	9	6.7	3334	PASS

m/z	Abundance
36.00	654.0
37.00	2719.0
38.00	2773.0
39.00	1279.0
39.90	367.0
44.00	725.0
45.00	440.0
46.90	575.0
48.00	386.0
49.10	2556.0
50.10	10915.0
51.00	3061.0
52.00	192.0
52.90	120.0
55.00	240.0
56.00	923.0
57.00	1655.0
59.90	504.0
61.00	3097.0
62.00	2976.0
63.00	2608.0
64.00	399.0
65.00	859.0
66.10	107.0
66.90	157.0
68.00	5522.0
69.00	6325.0
70.00	526.0
72.10	287.0
73.00	2492.0
74.00	9871.0
75.00	28120.0
76.10	2463.0
77.00	309.0
78.90	2373.0
79.90	571.0
80.90	2291.0
81.90	433.0
86.00	116.0
87.00	2283.0
88.00	2502.0
91.10	273.0
92.00	1722.0
93.00	2770.0
94.00	6513.0
95.10	57384.0
96.10	3946.0
103.80	291.0
105.90	161.0
115.80	291.0
116.90	403.0
117.90	344.0
118.90	343.0
128.00	187.0
129.80	153.0
131.00	125.0
136.80	117.0
141.00	668.0
142.90	849.0
145.00	314.0
147.90	120.0
154.80	145.0
156.80	132.0
171.20	205.0
171.90	1013.0
174.00	50488.0
175.00	3820.0
176.00	48560.0
177.00	3296.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	654.0
37.00	2719.0
38.00	2773.0
39.00	1279.0
39.90	367.0
44.00	725.0
45.00	440.0
46.90	575.0
48.00	386.0
49.10	2556.0
50.10	10915.0
51.00	3061.0
52.00	192.0
52.90	120.0
55.00	240.0
56.00	923.0
57.00	1655.0
59.90	504.0
61.00	3097.0
62.00	2976.0
63.00	2608.0
64.00	399.0
65.00	859.0
66.10	107.0
66.90	157.0
68.00	5522.0
69.00	6325.0
70.00	526.0
72.10	287.0
73.00	2492.0
74.00	9871.0
75.00	28120.0
76.10	2463.0
77.00	309.0
78.90	2373.0
79.90	571.0
80.90	2291.0
81.90	433.0
86.00	116.0
87.00	2283.0
88.00	2502.0
91.10	273.0
92.00	1722.0
93.00	2770.0
94.00	6513.0
95.10	57384.0
96.10	3946.0
103.80	291.0
105.90	161.0
115.80	291.0
116.90	403.0
117.90	344.0
118.90	343.0
128.00	187.0
129.80	153.0
131.00	125.0
136.80	117.0
141.00	668.0
142.90	849.0
145.00	314.0
147.90	120.0
154.80	145.0
156.80	132.0
171.20	205.0
171.90	1013.0
174.00	50488.0
175.00	3820.0
176.00	48560.0
177.00	3296.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	614.0
37.00	2807.0
38.00	2389.0
39.00	1058.0
39.90	315.0
44.10	672.0
45.10	374.0
47.00	595.0
47.90	261.0
49.10	2424.0
50.00	10114.0
51.00	3242.0
52.10	235.0
54.90	206.0
56.00	979.0
57.00	1756.0
60.00	606.0
61.00	2914.0
62.00	2653.0
63.00	2712.0
64.00	382.0
65.00	938.0
66.20	100.0
66.80	151.0
68.00	5213.0
69.00	5634.0
70.10	539.0
72.00	349.0
73.00	2332.0
74.00	9188.0
75.00	28144.0
76.00	2603.0
76.90	343.0
77.80	206.0
78.90	2283.0
79.90	484.0
80.90	2182.0
81.90	486.0
86.90	2154.0
88.00	2569.0
90.90	287.0
92.00	1880.0
93.00	2824.0
94.00	6872.0
95.10	56624.0
96.10	3589.0
96.90	103.0
103.80	290.0
104.90	117.0
105.80	171.0
114.80	103.0
115.90	242.0
117.00	463.0
117.80	323.0
118.90	465.0
127.70	210.0
129.90	286.0
136.80	182.0
140.90	484.0
141.80	104.0
142.90	991.0
144.90	308.0
147.90	127.0
154.90	200.0
170.80	245.0
172.00	1258.0
173.00	987.0
174.00	51136.0
175.00	4157.0
176.00	49448.0
176.90	3282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Scan 2848 (10.247 min): VU033835.D
BFB03

m/z	Abundance
39.80	271.0
43.90	306.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03