


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081920\
 Data File : VU039896.D
 Acq On : 19 Aug 2020 09:01
 Operator : SY/MD
 Sample : BFB16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Aug 20 08:13:41 2020

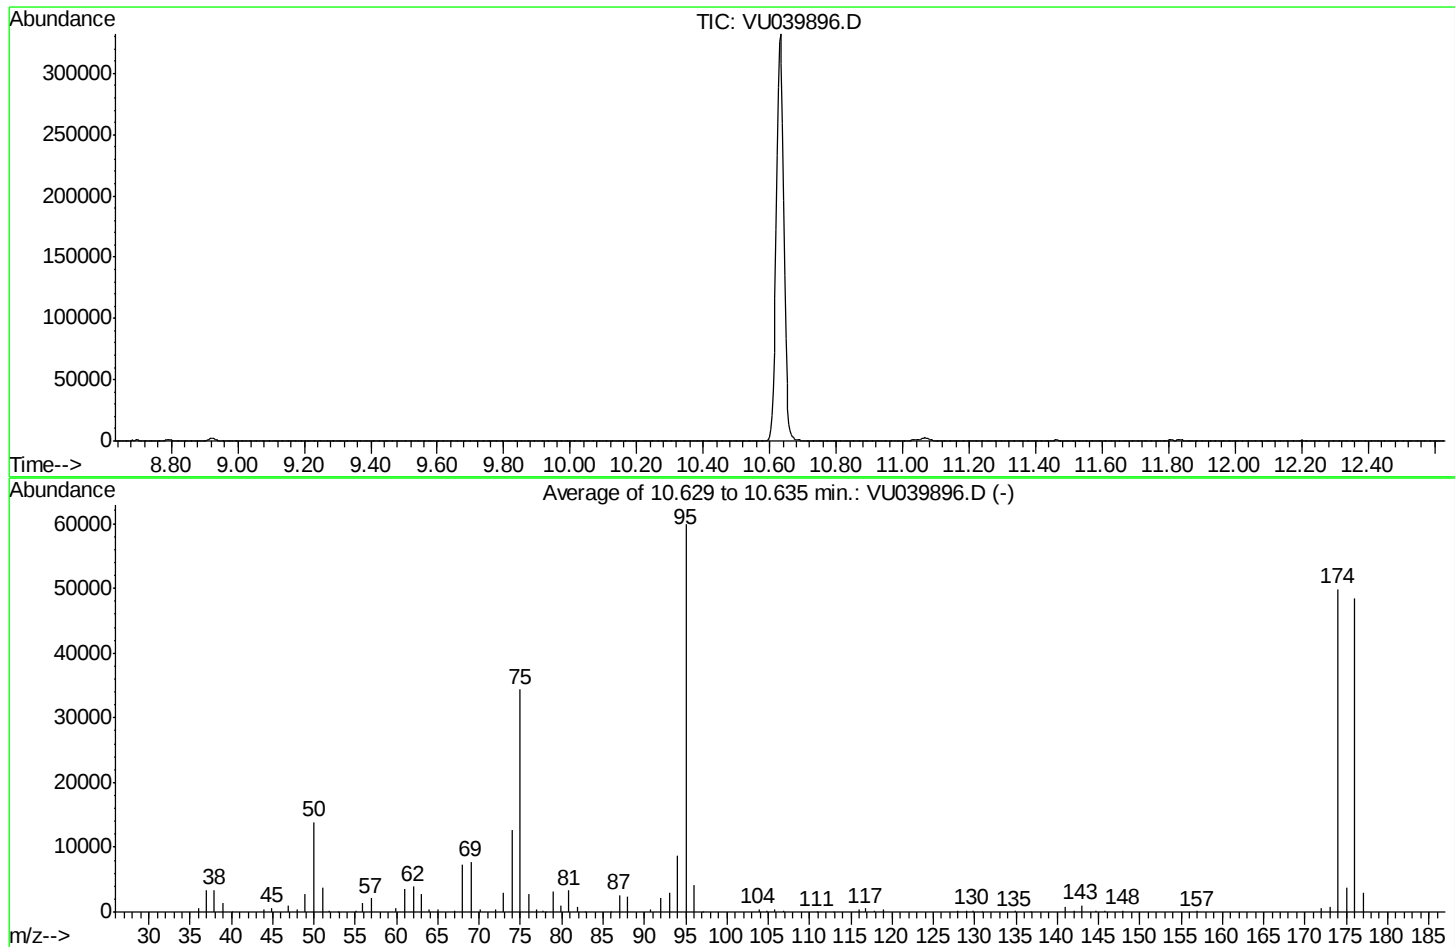

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	13934	PASS
75	95	30	80	57.3	34330	PASS
95	95	100	100	100.0	59888	PASS
96	95	5	9	6.9	4147	PASS
173	174	0.00	2	1.6	776	PASS
174	95	50	120	83.2	49845	PASS
175	174	5	9	7.4	3692	PASS
176	174	95	101	97.1	48392	PASS
177	176	5	9	6.3	3065	PASS

m/z	Abundance
35.90	568.0
36.90	3532.0
37.90	3656.0
38.90	1532.0
43.90	720.0
44.90	730.0
46.90	929.0
48.00	348.0
48.90	3084.0
50.00	14200.0
51.00	3936.0
51.90	332.0
52.90	100.0
55.10	260.0
55.90	1406.0
56.90	2204.0
60.00	529.0
61.00	3885.0
62.00	4206.0
63.00	2833.0
63.90	363.0
65.10	509.0
67.00	228.0
68.00	7446.0
69.00	8023.0
70.10	497.0
72.00	293.0
72.90	3144.0
74.00	12668.0
75.00	34800.0
76.00	2730.0
76.90	438.0
77.60	169.0
78.00	195.0
78.90	3352.0
79.90	1082.0
80.80	3252.0
81.90	750.0
82.90	121.0
86.00	105.0
86.90	2640.0
88.00	2397.0
90.80	401.0
91.90	2422.0
93.00	3123.0
94.00	8709.0
95.00	60976.0
96.00	4332.0
97.00	107.0
103.80	404.0
104.80	199.0
105.80	348.0
106.80	147.0
116.00	265.0
116.80	552.0
118.00	237.0
118.90	484.0
128.00	225.0
129.00	133.0
129.80	229.0
134.90	106.0
136.80	109.0
141.00	780.0
142.10	103.0
142.90	1090.0
144.70	150.0
145.70	108.0
148.00	211.0
157.00	108.0
171.90	781.0
173.00	767.0
174.00	49472.0
175.00	3719.0
176.00	47416.0
177.00	3114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	560.0
36.90	3381.0
38.00	3497.0
38.90	1500.0
40.00	114.0
43.90	693.0
44.90	616.0
46.90	1040.0
48.00	392.0
49.00	2929.0
50.00	14430.0
51.00	3911.0
51.90	318.0
55.10	239.0
55.90	1422.0
56.90	2214.0
60.00	606.0
61.00	3702.0
62.00	4085.0
63.00	2927.0
63.90	310.0
65.10	498.0
67.00	262.0
68.00	7675.0
69.00	8047.0
70.10	517.0
71.90	333.0
73.00	3164.0
74.00	12903.0
75.00	35424.0
76.00	2922.0
76.90	486.0
77.60	197.0
78.90	3222.0
79.80	1035.0
80.90	3480.0
81.90	742.0
87.00	2778.0
88.00	2524.0
90.80	438.0
91.90	2390.0
93.00	3171.0
94.00	8924.0
95.00	61736.0
96.00	4303.0
97.10	101.0
103.80	406.0
104.90	191.0
105.80	379.0
106.80	147.0
112.80	125.0
116.00	336.0
116.80	559.0
117.80	201.0
119.00	482.0
127.90	194.0
128.90	185.0
129.70	264.0
130.90	103.0
134.90	136.0
141.00	754.0
142.10	127.0
142.90	1043.0
144.70	167.0
145.70	116.0
148.00	235.0
156.90	170.0
171.90	686.0
173.00	828.0
174.00	51352.0
175.00	3760.0
176.00	49912.0
177.00	3186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	427.0
37.00	3081.0
38.00	3107.0
38.90	1311.0
40.00	146.0
44.00	610.0
44.90	474.0
46.90	918.0
47.90	404.0
49.00	2529.0
50.00	13174.0
51.00	3587.0
51.90	212.0
55.10	164.0
55.90	1229.0
56.90	2055.0
59.90	648.0
60.90	3187.0
62.00	3478.0
63.00	2729.0
63.80	258.0
65.00	431.0
67.10	224.0
68.00	6836.0
69.00	7126.0
70.00	486.0
71.90	341.0
73.00	2897.0
74.00	12130.0
75.00	32768.0
76.00	2855.0
76.90	456.0
77.70	204.0
78.90	2951.0
79.90	1014.0
80.90	3346.0
81.90	663.0
87.00	2576.0
88.00	2454.0
90.80	412.0
91.90	1965.0
93.00	2888.0
94.00	8349.0
95.00	56952.0
96.00	3806.0
103.90	388.0
104.90	134.0
105.70	370.0
106.80	100.0
110.90	107.0
112.90	143.0
116.00	354.0
116.80	495.0
117.80	178.0
119.00	437.0
127.80	183.0
128.90	179.0
129.70	227.0
134.90	133.0
141.00	712.0
142.00	156.0
142.90	904.0
144.70	144.0
145.70	106.0
148.00	202.0
156.90	195.0
171.90	597.0
173.00	735.0
174.00	48712.0
175.00	3597.0
176.00	47848.0
177.00	2896.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
44.00	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16