
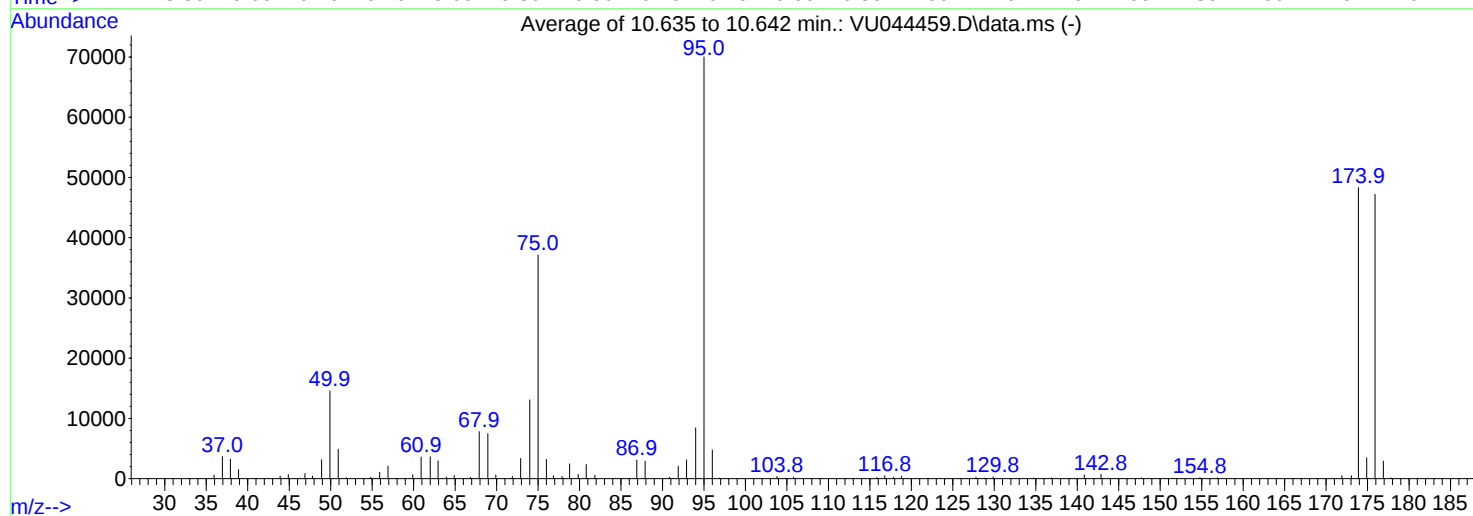


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081921\
 Data File : VU044459.D
 Acq On : 19 Aug 2021 09:01
 Operator : SY/MD
 Sample : BFB007
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB007

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Aug 20 05:12:49 2021

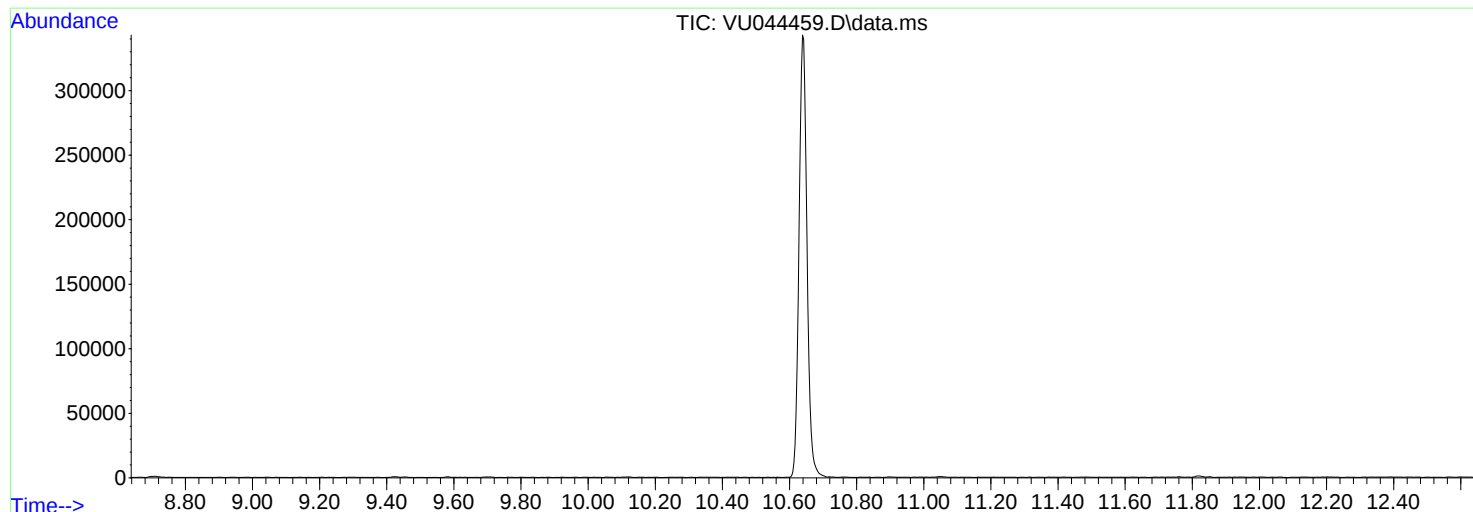

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	14559	PASS
75	95	30	80	53.0	37128	PASS
95	95	100	100	100.0	70019	PASS
96	95	5	9	6.8	4759	PASS
173	174	0.00	2	1.0	468	PASS
174	95	50	120	69.0	48328	PASS
175	174	5	9	7.1	3445	PASS
176	174	95	101	97.7	47203	PASS
177	176	5	9	6.2	2935	PASS

m/z	Abundance
35.90	633.0
37.00	3784.0
37.90	3334.0
38.90	1595.0
39.80	183.0
43.90	785.0
44.90	674.0
46.90	889.0
47.80	448.0
48.90	3207.0
49.90	14966.0
50.90	5066.0
51.90	200.0
54.90	258.0
55.90	1095.0
56.90	2173.0
57.90	100.0
59.90	678.0
60.90	3700.0
62.00	3744.0
63.00	3001.0
63.90	302.0
64.90	529.0
66.90	236.0
67.90	8062.0
69.00	7647.0
69.90	656.0
71.90	378.0
72.90	3457.0
74.00	13462.0
75.00	38384.0
76.00	3300.0
76.90	490.0
77.90	396.0
78.80	2551.0
79.90	689.0
80.80	2419.0
81.80	558.0
86.90	3184.0
87.90	2916.0
90.80	263.0
91.90	2140.0
92.90	3197.0
94.00	8700.0
95.00	72104.0
96.00	4915.0
96.90	111.0
103.80	354.0
104.90	103.0
105.80	277.0
115.80	195.0
116.80	531.0
117.90	235.0
118.80	413.0
127.80	267.0
128.80	103.0
129.80	283.0
130.80	106.0
134.80	120.0
136.90	158.0
140.80	644.0
142.90	745.0
144.80	107.0
147.70	143.0
154.80	193.0
156.90	138.0
171.90	529.0
173.10	483.0
173.90	49736.0
174.90	3546.0
175.90	48912.0
176.90	3007.0
177.80	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	632.0
36.90	3703.0
37.90	3229.0
38.90	1552.0
39.90	173.0
43.90	728.0
44.90	668.0
46.90	877.0
47.80	443.0
48.90	3048.0
49.90	14829.0
50.90	4925.0
51.90	187.0
54.80	268.0
55.90	1094.0
56.90	2167.0
59.90	621.0
60.90	3641.0
62.00	3534.0
62.90	3014.0
63.90	353.0
64.90	515.0
66.90	252.0
67.90	7935.0
68.90	7446.0
69.90	579.0
71.90	396.0
72.90	3404.0
74.00	13261.0
75.00	37448.0
76.00	3304.0
76.90	475.0
77.90	354.0
78.80	2428.0
79.80	700.0
80.80	2465.0
81.80	548.0
85.90	111.0
86.90	3138.0
87.90	3182.0
90.90	238.0
91.90	2054.0
92.90	3115.0
94.00	8262.0
95.00	71432.0
96.00	4793.0
96.90	100.0
103.80	397.0
104.80	116.0
105.80	293.0
115.80	202.0
116.80	507.0
117.90	254.0
118.80	395.0
127.80	246.0
128.90	125.0
129.90	276.0
134.80	100.0
136.80	146.0
140.90	682.0
142.90	715.0
147.70	162.0
154.80	186.0
156.90	129.0
171.90	532.0
173.00	476.0
173.90	50032.0
174.90	3660.0
175.90	49008.0
176.90	3080.0
177.80	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
39.80	182.0
43.90	343.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.00	558.0
37.00	3517.0
37.90	3150.0
38.90	1420.0
39.80	180.0
43.90	820.0
44.90	614.0
46.90	816.0
47.80	363.0
48.90	3119.0
49.90	13881.0
50.90	4674.0
51.90	197.0
54.80	226.0
55.90	1035.0
56.90	1982.0
59.90	664.0
60.90	3454.0
62.00	3647.0
63.00	2843.0
64.00	263.0
64.90	483.0
66.80	178.0
67.90	7453.0
68.90	7269.0
69.90	642.0
71.90	353.0
72.90	3196.0
74.00	12447.0
75.00	35552.0
76.00	3005.0
76.80	475.0
77.90	367.0
78.80	2358.0
79.90	651.0
80.80	2135.0
81.90	539.0
86.90	2947.0
87.90	2581.0
90.80	248.0
91.90	2004.0
92.90	2983.0
94.00	8271.0
95.00	66520.0
96.00	4570.0
96.90	123.0
103.80	287.0
105.80	262.0
115.90	182.0
116.80	491.0
117.80	205.0
118.80	368.0
127.80	251.0
128.80	113.0
129.80	286.0
134.70	116.0
136.90	138.0
140.80	589.0
142.80	692.0
147.80	122.0
154.80	171.0
156.90	116.0
171.90	456.0
173.10	445.0
173.90	45216.0
174.90	3130.0
175.90	43688.0
176.90	2717.0
177.80	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007