

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081924\
 Data File : VU060481.D
 Acq On : 19 Aug 2024 11:23
 Operator : MD/SY
 Sample : VU0819WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 20 06:31:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 17 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	4972	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	7477	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	2237	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	4708	0.582	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	116.000%
4) 1,2-Dichloroethane-d4	5.709	65	2485	0.580	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
7) 1,2-Dichloropropane-d6	6.687	67	2722	0.586	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	118.000%
8) Toluene-d8	7.888	98	5344	0.556	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
10) 1,1,2,2-Tetrachloroeth...	10.746	84	2413	0.593	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	118.000%
Target Compounds						
12) 1,2,3-Trichloropropane	10.643	75	73	0.028	ug/L	Qvalue # 41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081924\
Data File : VU060481.D
Acq On : 19 Aug 2024 11:23
Operator : MD/SY
Sample : VU0819WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Aug 20 06:31:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 17 05:03:57 2024
Response via : Initial Calibration

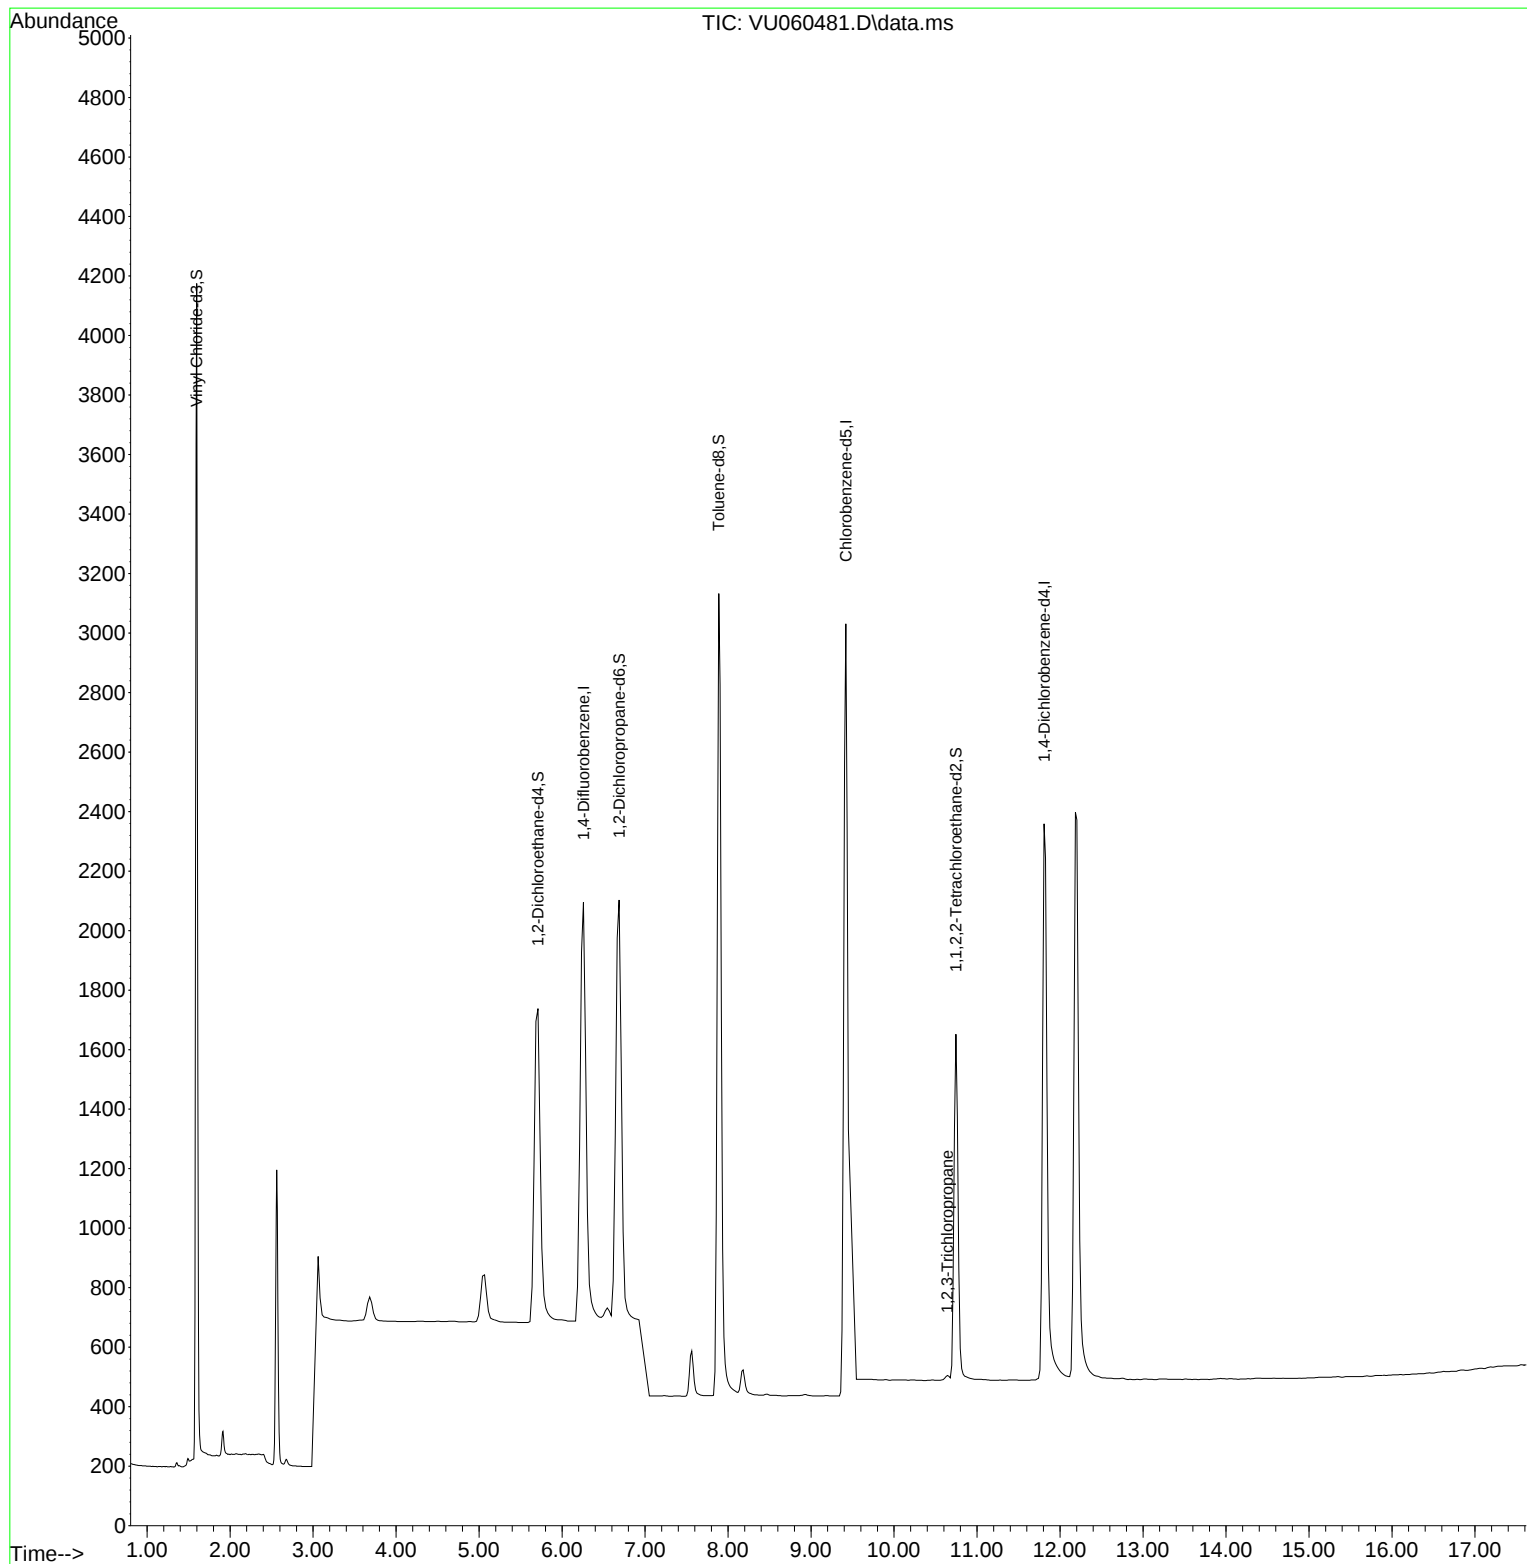

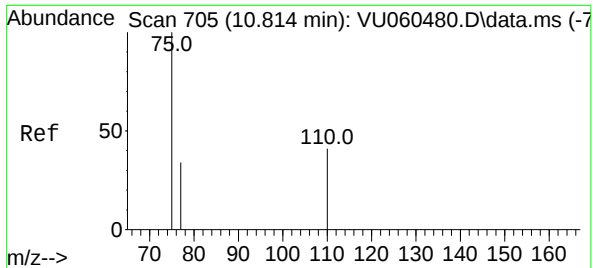

#12
 1,2,3-Trichloropropane
 Concen: 0.028 ug/L
 RT: 10.643 min Scan# 61
 Delta R.T. -0.171 min
 Lab File: VU060481.D
 Acq: 19 Aug 2024 11:23

Instrument :
 MSVOA_U
 ClientSampleId :

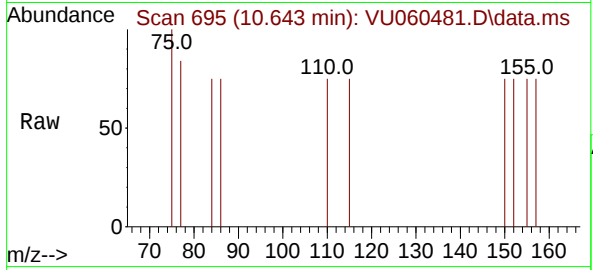

Tgt Ion: 75	Resp:	73
Ion	Ratio	Lower Upper
75	100	
110	0.0	32.4 48.6#
77	4.1	26.0 39.0#

