


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081924\
Data File : VU060479.D
Acq On : 19 Aug 2024 09:36
Operator : MD/SY
Sample : BFB012
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB012

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081624.M
Title : TRACE VOA SOM01.0
Last Update : Sat Aug 17 05:03:57 2024

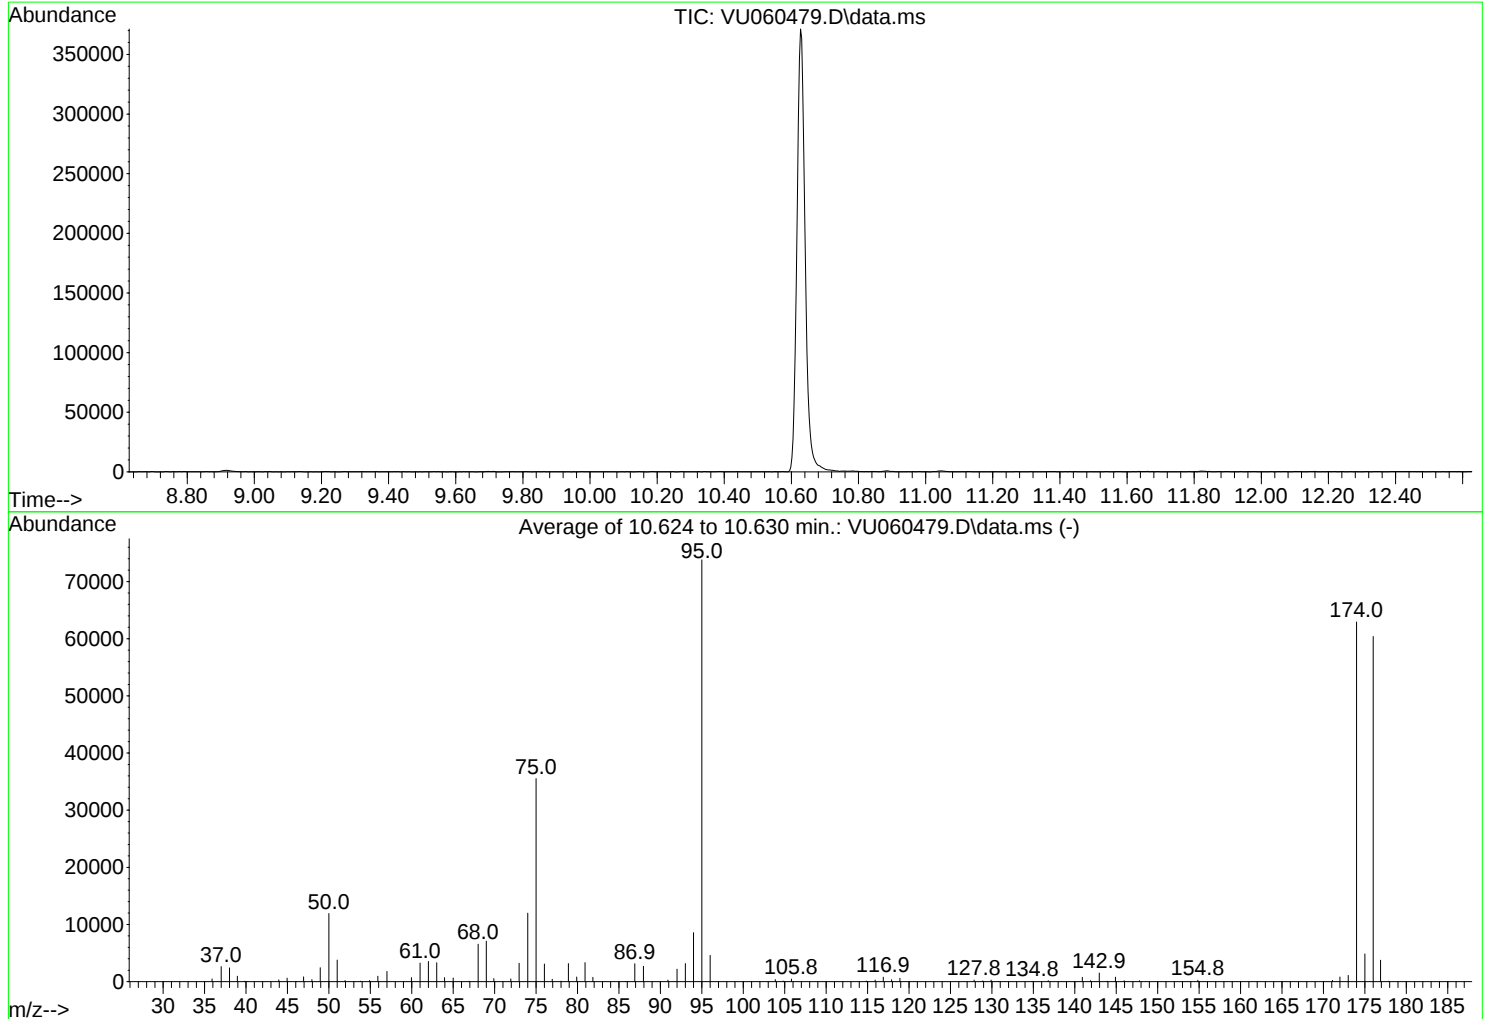

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	11943	PASS
75	95	30	80	48.1	35533	PASS
95	95	100	100	100.0	73800	PASS
96	95	5	9	6.2	4607	PASS
173	174	0.00	2	1.7	1086	PASS
174	95	50	120	85.3	62928	PASS
175	174	5	9	7.7	4852	PASS
176	174	95	101	95.9	60376	PASS
177	176	5	9	6.2	3764	PASS

m/z	Abundance
43.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	411.0
37.00	2660.0
38.00	2425.0
39.00	967.0
39.80	153.0
44.00	454.0
44.90	586.0
46.90	836.0
47.90	396.0
49.00	2330.0
50.00	11263.0
51.00	3538.0
51.90	212.0
53.80	107.0
55.00	199.0
55.90	911.0
57.00	1843.0
60.00	677.0
61.00	3154.0
62.00	3437.0
63.00	3333.0
64.00	701.0
65.00	622.0
68.00	6276.0
69.00	6940.0
69.90	504.0
71.90	439.0
72.90	3182.0
74.00	11553.0
75.00	34256.0
76.00	3131.0
77.00	383.0
78.90	3045.0
79.90	744.0
80.90	3357.0
81.80	738.0
86.10	100.0
86.90	2932.0
87.90	2700.0
90.90	276.0
92.00	2050.0
93.00	3004.0
94.00	8273.0
95.00	71872.0
96.00	4533.0
103.80	322.0
104.90	119.0
105.80	389.0
114.90	114.0
115.90	226.0
116.90	711.0
117.90	262.0
118.90	575.0
127.90	267.0
128.90	160.0
129.90	297.0
136.80	142.0
140.90	748.0
141.90	162.0
142.90	1550.0
144.90	766.0
146.00	118.0
147.80	163.0
154.90	252.0
171.10	201.0
172.00	817.0
173.00	1070.0
174.00	59520.0
175.00	4648.0
176.00	57352.0
176.90	3527.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	459.0
37.00	2705.0
38.00	2525.0
38.90	946.0
39.90	134.0
44.00	477.0
44.90	664.0
46.90	915.0
47.90	375.0
48.90	2446.0
50.00	12273.0
51.00	3880.0
51.90	201.0
53.80	116.0
54.90	193.0
55.90	1009.0
57.00	1847.0
59.90	687.0
61.00	3349.0
62.00	3652.0
63.00	3396.0
63.90	741.0
65.00	673.0
66.90	108.0
68.00	6737.0
69.00	7268.0
69.90	554.0
72.00	507.0
73.00	3301.0
74.00	12385.0
75.00	36640.0
76.00	3167.0
76.90	433.0
78.90	3237.0
79.90	846.0
80.90	3412.0
81.80	757.0
86.90	3201.0
87.90	2777.0
90.90	300.0
92.00	2297.0
93.00	3266.0
94.00	8758.0
95.00	76200.0
96.00	4742.0
103.90	381.0
104.80	117.0
105.80	471.0
114.80	138.0
115.90	285.0
116.90	812.0
117.90	351.0
118.90	620.0
127.90	267.0
128.90	142.0
129.90	281.0
134.80	102.0
136.80	185.0
140.90	785.0
141.90	185.0
143.00	1552.0
143.90	114.0
144.90	799.0
146.00	158.0
147.80	165.0
154.80	261.0
171.10	243.0
172.00	841.0
173.00	1117.0
174.00	65096.0
175.00	5026.0
176.00	62192.0
176.90	3896.0
177.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	542.0
37.00	2525.0
38.00	2256.0
38.90	910.0
40.10	128.0
44.00	481.0
45.00	632.0
46.10	119.0
47.00	777.0
48.00	333.0
48.90	2495.0
50.00	12293.0
51.00	3897.0
52.00	183.0
54.80	221.0
55.90	973.0
57.00	1699.0
59.90	706.0
61.00	3242.0
62.00	3516.0
63.00	3179.0
63.90	702.0
65.00	675.0
66.90	164.0
68.00	6637.0
69.00	7029.0
69.90	571.0
72.00	465.0
73.00	3163.0
74.00	12002.0
75.00	35704.0
76.00	2934.0
76.90	430.0
78.00	248.0
78.90	3242.0
79.90	860.0
80.90	3240.0
81.90	740.0
85.80	105.0
86.90	3300.0
88.00	2614.0
90.90	293.0
92.00	2231.0
93.00	3199.0
94.00	8659.0
95.00	73328.0
96.00	4547.0
103.80	382.0
104.70	107.0
105.80	467.0
114.80	128.0
115.90	322.0
116.90	871.0
117.90	425.0
118.90	563.0
127.80	290.0
128.90	123.0
129.90	246.0
130.80	125.0
134.90	108.0
136.80	176.0
139.90	122.0
140.90	753.0
141.90	167.0
143.00	1440.0
143.90	103.0
144.90	797.0
145.90	209.0
147.80	156.0
154.80	274.0
157.00	112.0
171.10	267.0
172.00	814.0
173.00	1071.0
174.00	64168.0
175.00	4881.0
176.00	61584.0
176.90	3870.0
177.90	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012