



Iodomethane

Response Ratio

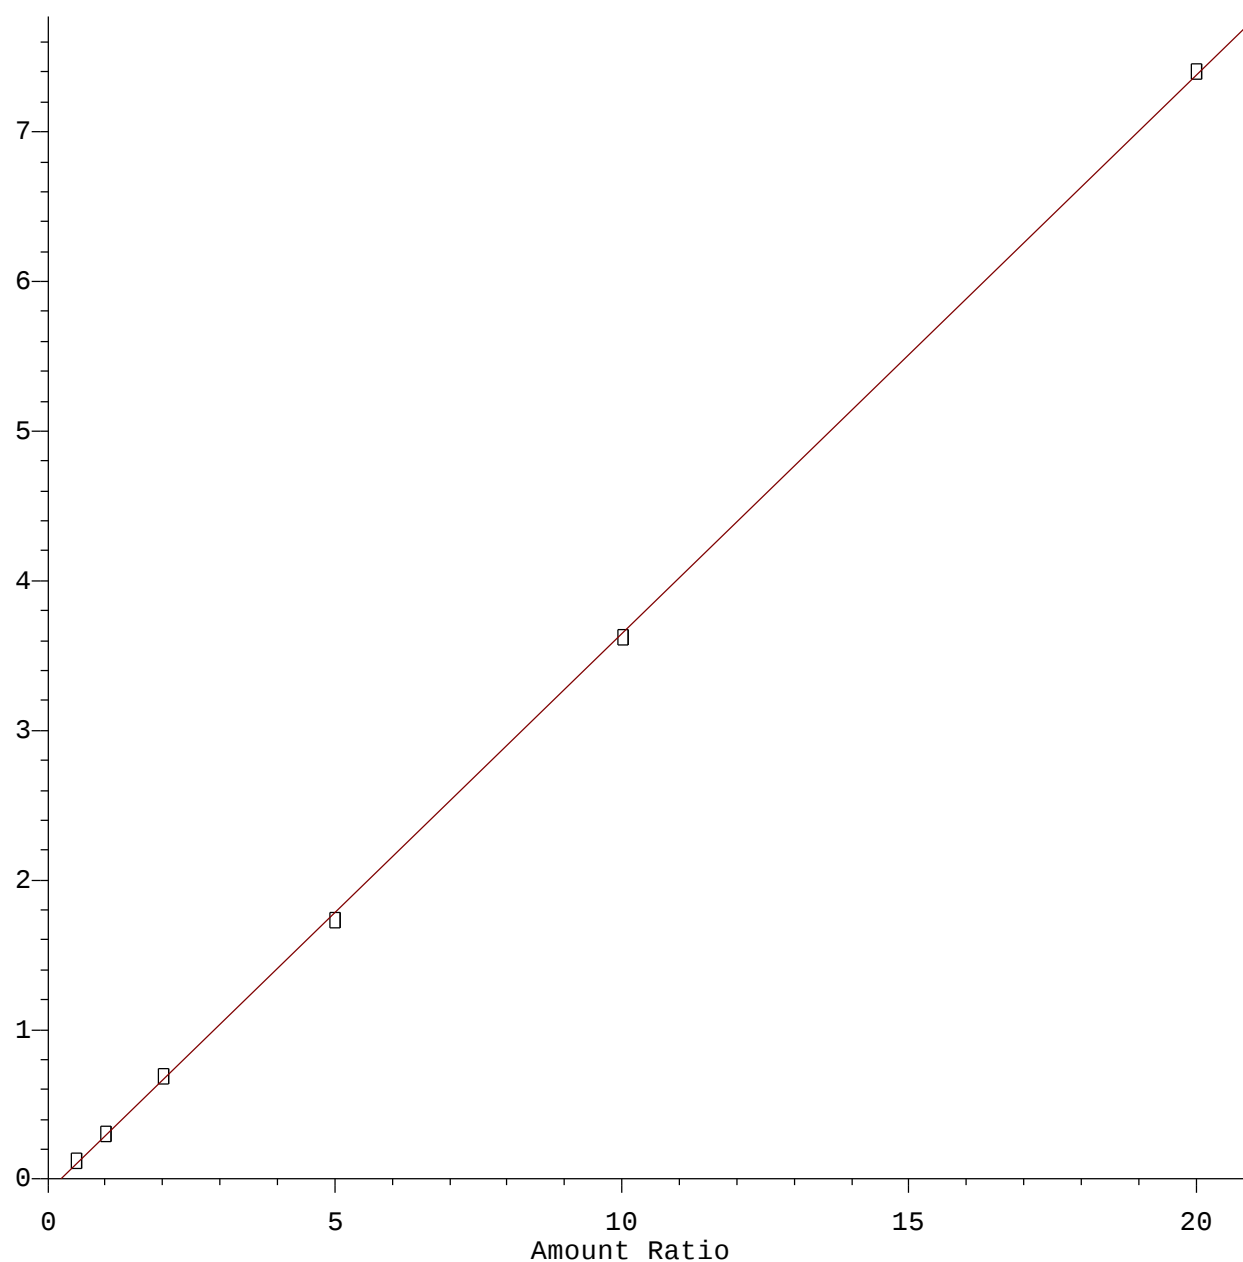

Resp Ratio = $3.73 \times 10^{-1} \times \text{Amt} - 8.75 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Calibration Table Last Updated: Tue Aug 21 11:25:08 2018

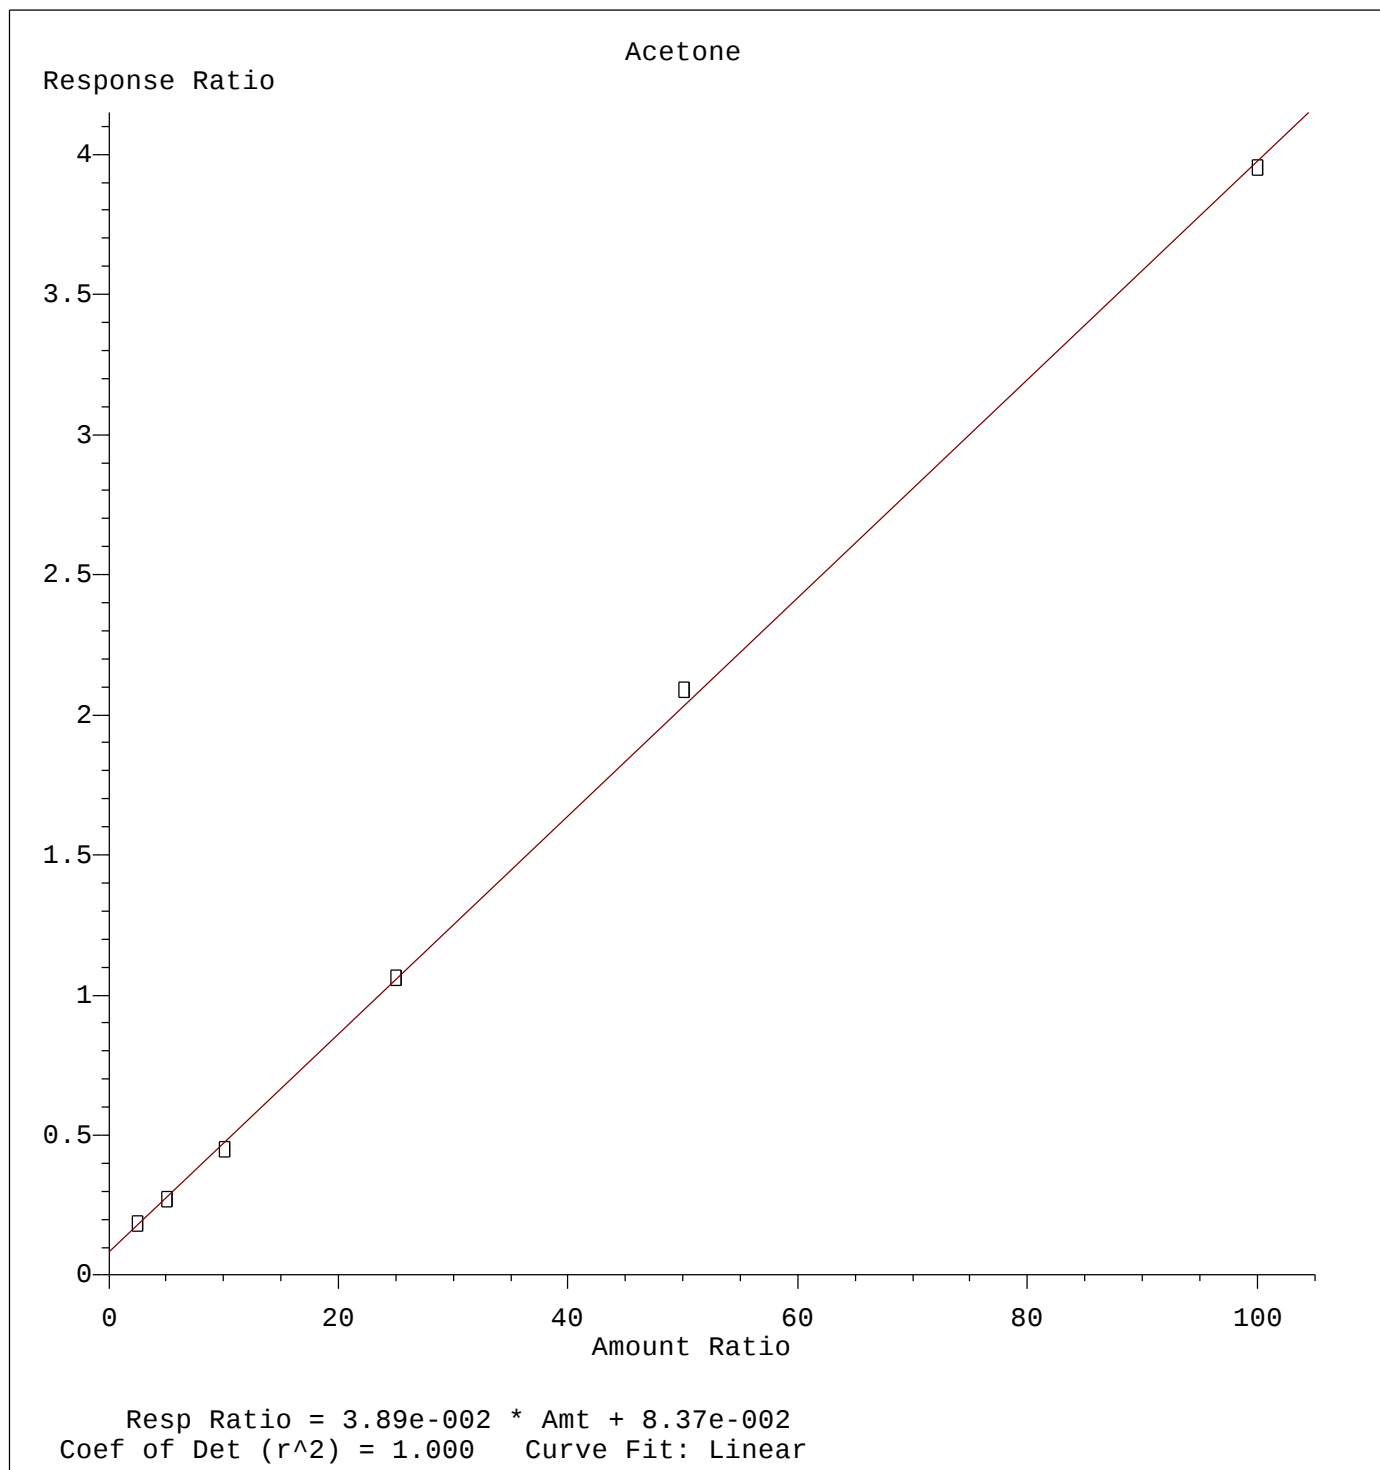

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Calibration Table Last Updated: Tue Aug 21 11:25:08 2018

Methylene Chloride

Response Ratio

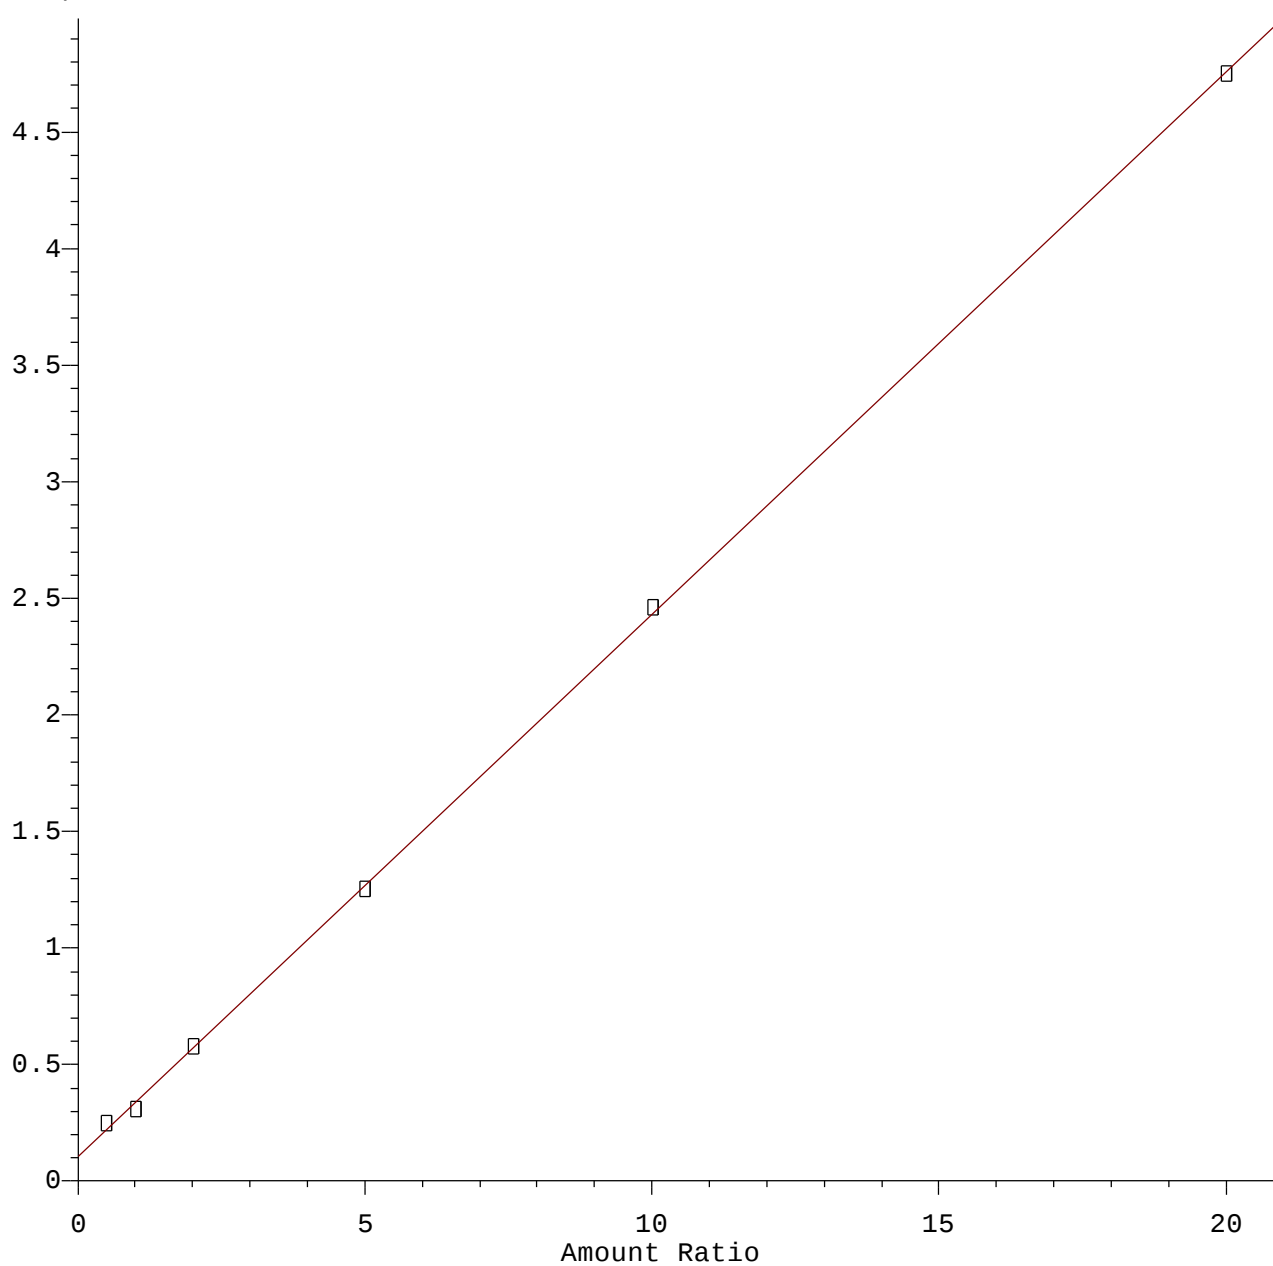


Resp Ratio = $2.32 \times 10^{-1} \times \text{Amt} + 1.07 \times 10^{-1}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Calibration Table Last Updated: Tue Aug 21 11:25:08 2018

t-1,4-Dichloro-2-butene

Response Ratio

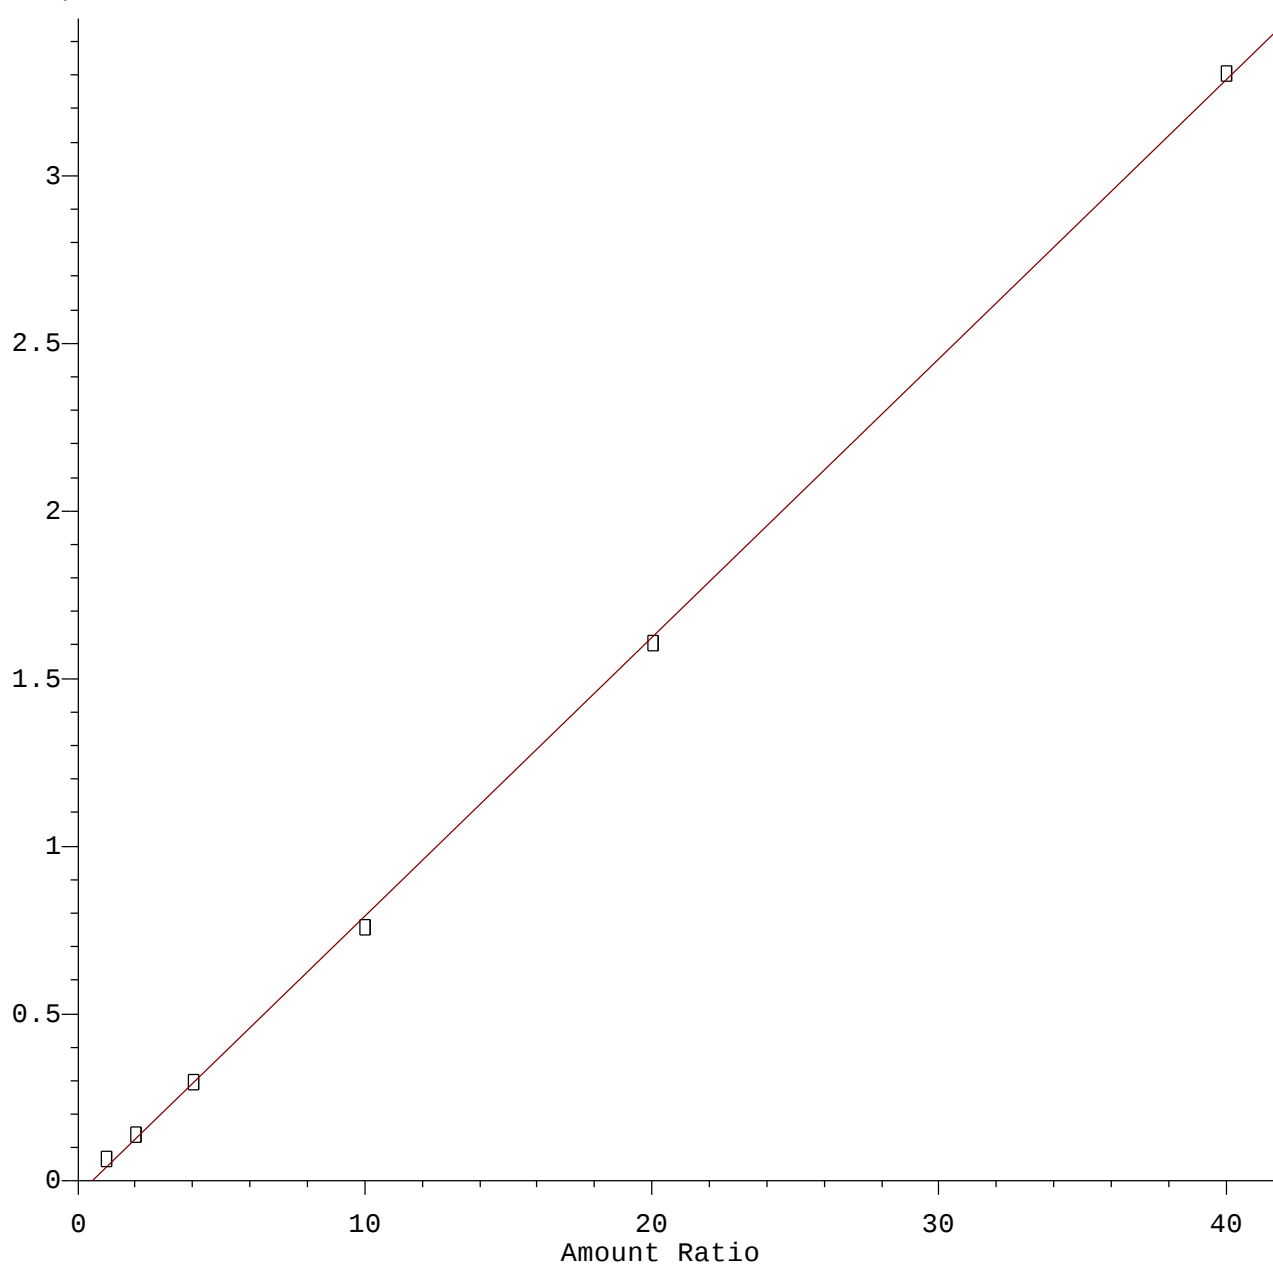

Resp Ratio = 8.32×10^{-2} * Amt - 4.08×10^{-2}
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Calibration Table Last Updated: Tue Aug 21 11:25:08 2018