

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082018\
Data File : VU026215.D
Acq On : 20 Aug 2018 17:58
Operator : MD/SY
Sample : J4045-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.291	515	529	550	rBV	372718	668400	20.51%	6.286%
2	3.005	733	751	776	rBV	981411	2124577	65.19%	19.982%
3	3.580	908	930	966	rBV	1331241	3259045	100.00%	30.652%
4	4.079	1062	1085	1110	rBV	175042	494548	15.17%	4.651%
5	5.587	1533	1554	1583	rBV	1374235	3018292	92.61%	28.387%
6	5.744	1591	1603	1617	rVB2	37723	74439	2.28%	0.700%
7	8.181	2348	2361	2373	rBV2	22297	44362	1.36%	0.417%
8	10.310	3013	3023	3037	rBV2	29132	44881	1.38%	0.422%
9	10.590	3095	3110	3128	rBV	540551	834017	25.59%	7.844%
10	11.863	3494	3506	3523	rBV	42172	69992	2.15%	0.658%




Sum of corrected areas: 10632553

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082018\
Data File : VU026215.D
Acq On : 20 Aug 2018 17:58
Operator : MD/SY
Sample : J4045-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U082018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

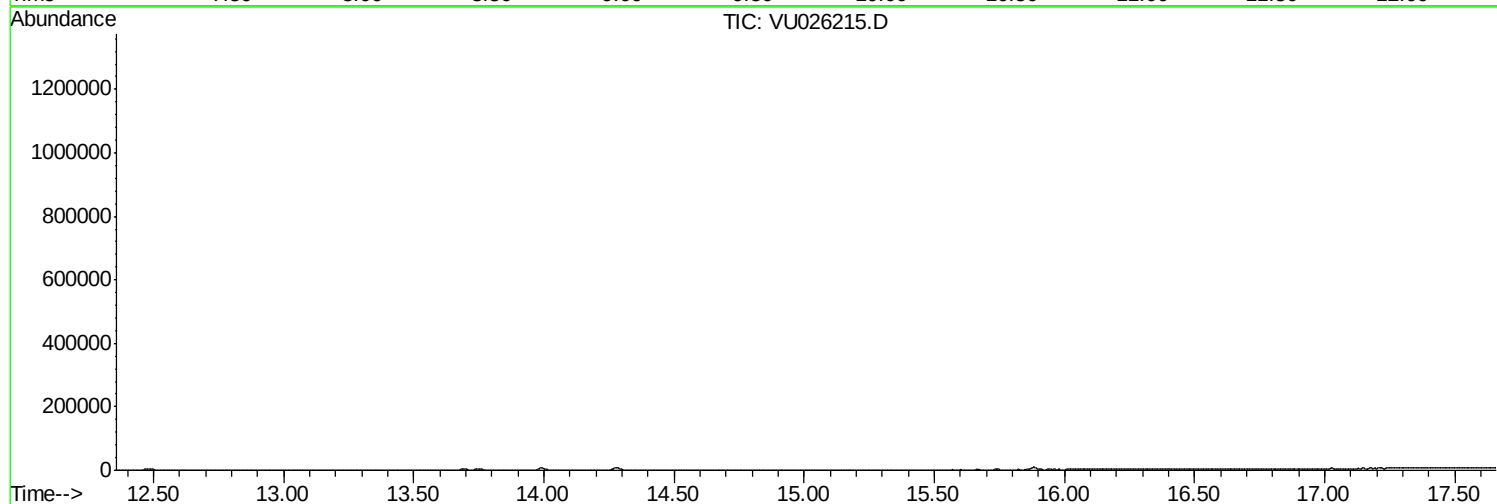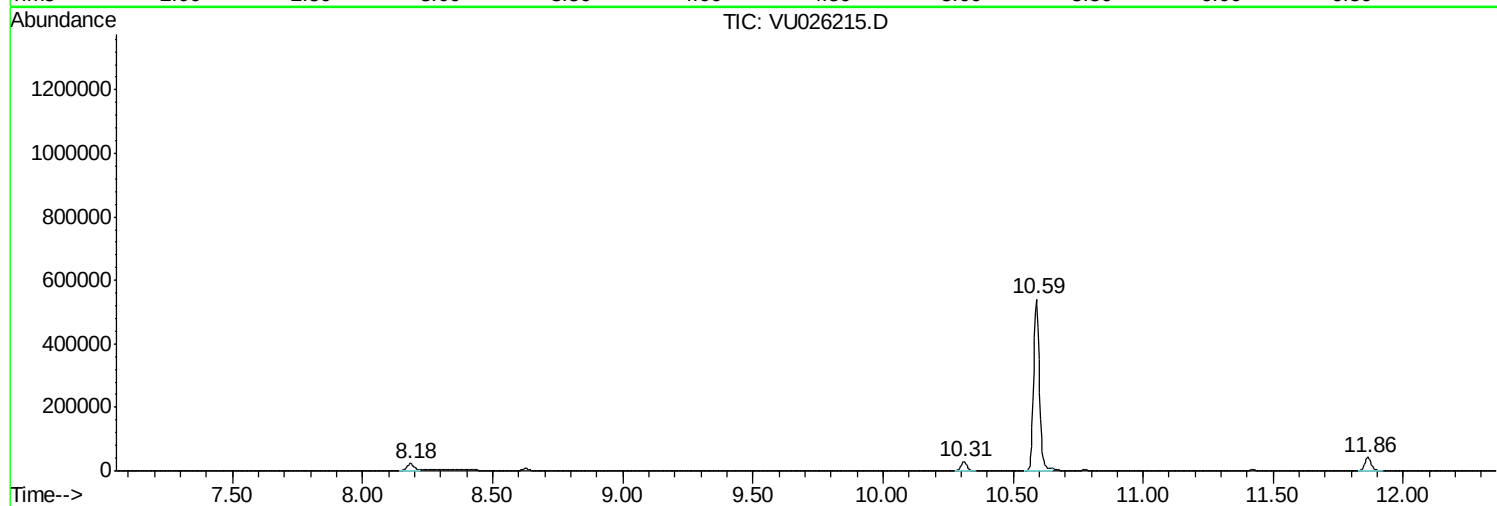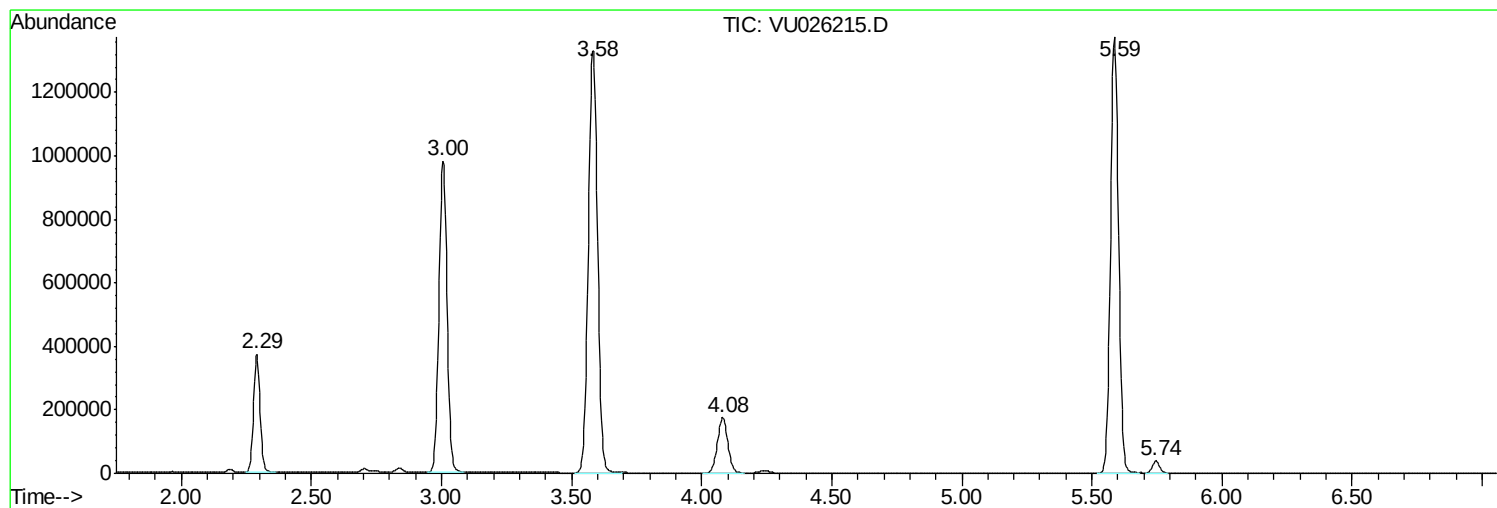

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082018\
Data File : VU026215.D
Acq On : 20 Aug 2018 17:58
Operator : MD/SY
Sample : J4045-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082018\
Data File : VU026215.D
Acq On : 20 Aug 2018 17:58
Operator : MD/SY
Sample : J4045-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc