


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082018\
 Data File : VU026198.D
 Acq On : 20 Aug 2018 10:33
 Operator : MD/SY
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Mon Aug 20 13:35:41 2018

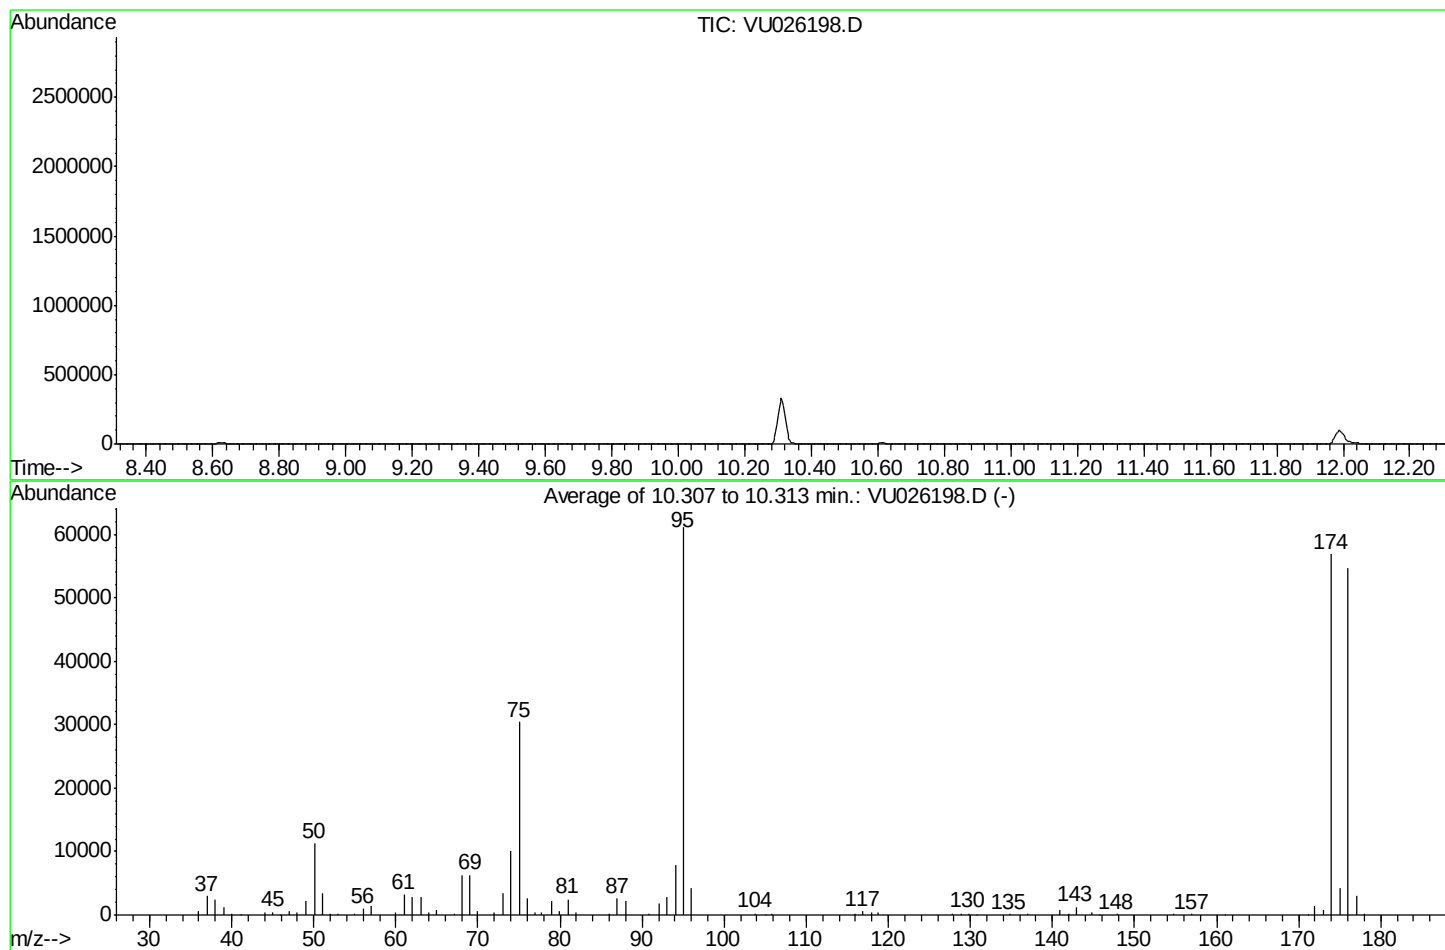

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3009

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	11245	PASS
75	95	30	60	49.8	30421	PASS
95	95	100	100	100.0	61125	PASS
96	95	5	9	7.0	4300	PASS
173	174	0.00	2	1.4	787	PASS
174	95	50	100	93.1	56888	PASS
175	174	5	9	7.6	4329	PASS
176	174	95	101	96.1	54672	PASS
177	176	5	9	5.7	3108	PASS