

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082019\
 Data File : VU033854.D
 Acq On : 20 Aug 2019 15:20
 Operator : JC/SP
 Sample : K4395-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AJ5

Quant Time: Aug 21 07:43:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082019WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 21 05:39:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	187336	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	189326	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	89181	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	66824	4.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.80%
7) Chloroethane-d5	1.67	69	61469	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.40%
11) 1,1-Dichloroethene-d2	2.26	63	113330	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	4.17	46	136443	43.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.22%
24) Chloroform-d	4.62	84	117891	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.29	65	64150	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
32) Benzene-d6	5.32	84	234450	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.31	67	74530	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.55	98	202172	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.84	79	26295	4.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.60%
46) 2-Hexanone-d5	8.30	63	84640	39.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.94%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	59479	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	11.84	152	82000	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Qvalue
13) Acetone	2.31	43	19922	8.234 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082019\
Data File : VU033854.D
Acq On : 20 Aug 2019 15:20
Operator : JC/SP
Sample : K4395-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AJ5

Quant Time: Aug 21 07:43:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 21 05:39:59 2019
Response via : Initial Calibration

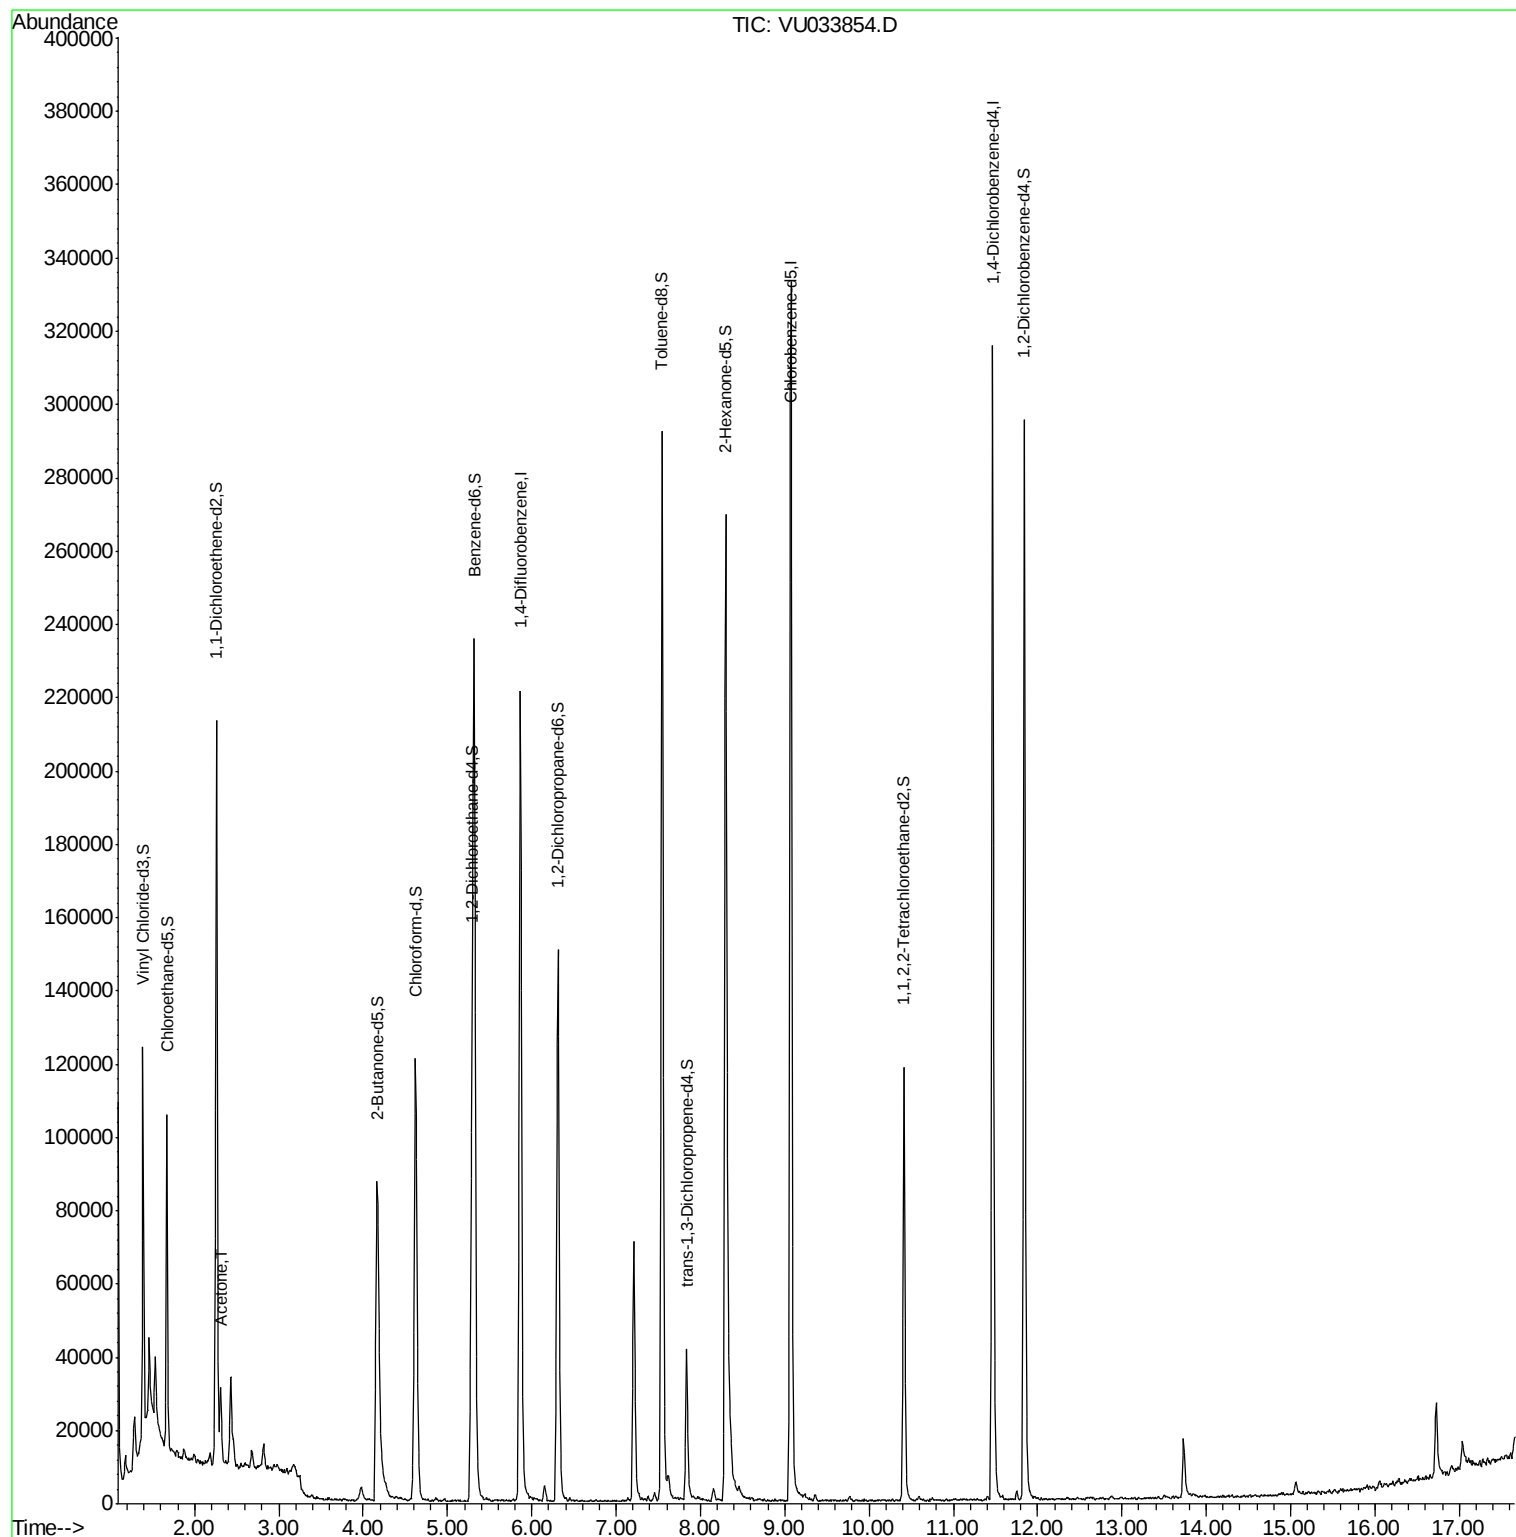

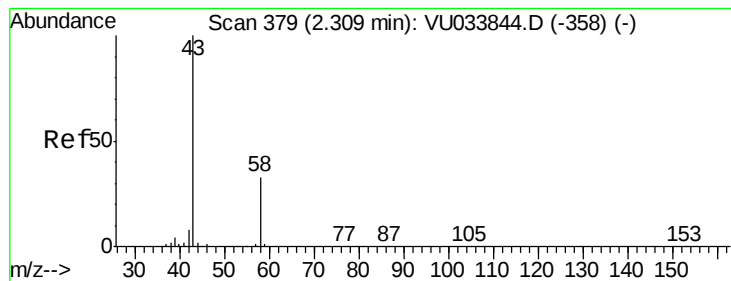

#13
 Acetone
 Concen: 8.234 ug/L
 RT: 2.31 min Scan# 379
 Delta R.T. -0.00 min
 Lab File: VU033854.D
 Acq: 20 Aug 2019 15:20

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AJ5

Tgt Ion: 43 Resp: 19922
 Ion Ratio Lower Upper
 43 100
 58 34.8 0.0 65.4

