


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082019\
 Data File : VU033841.D
 Acq On : 20 Aug 2019 09:29
 Operator : JC/SP
 Sample : BFB04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082019WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 21 05:39:59 2019

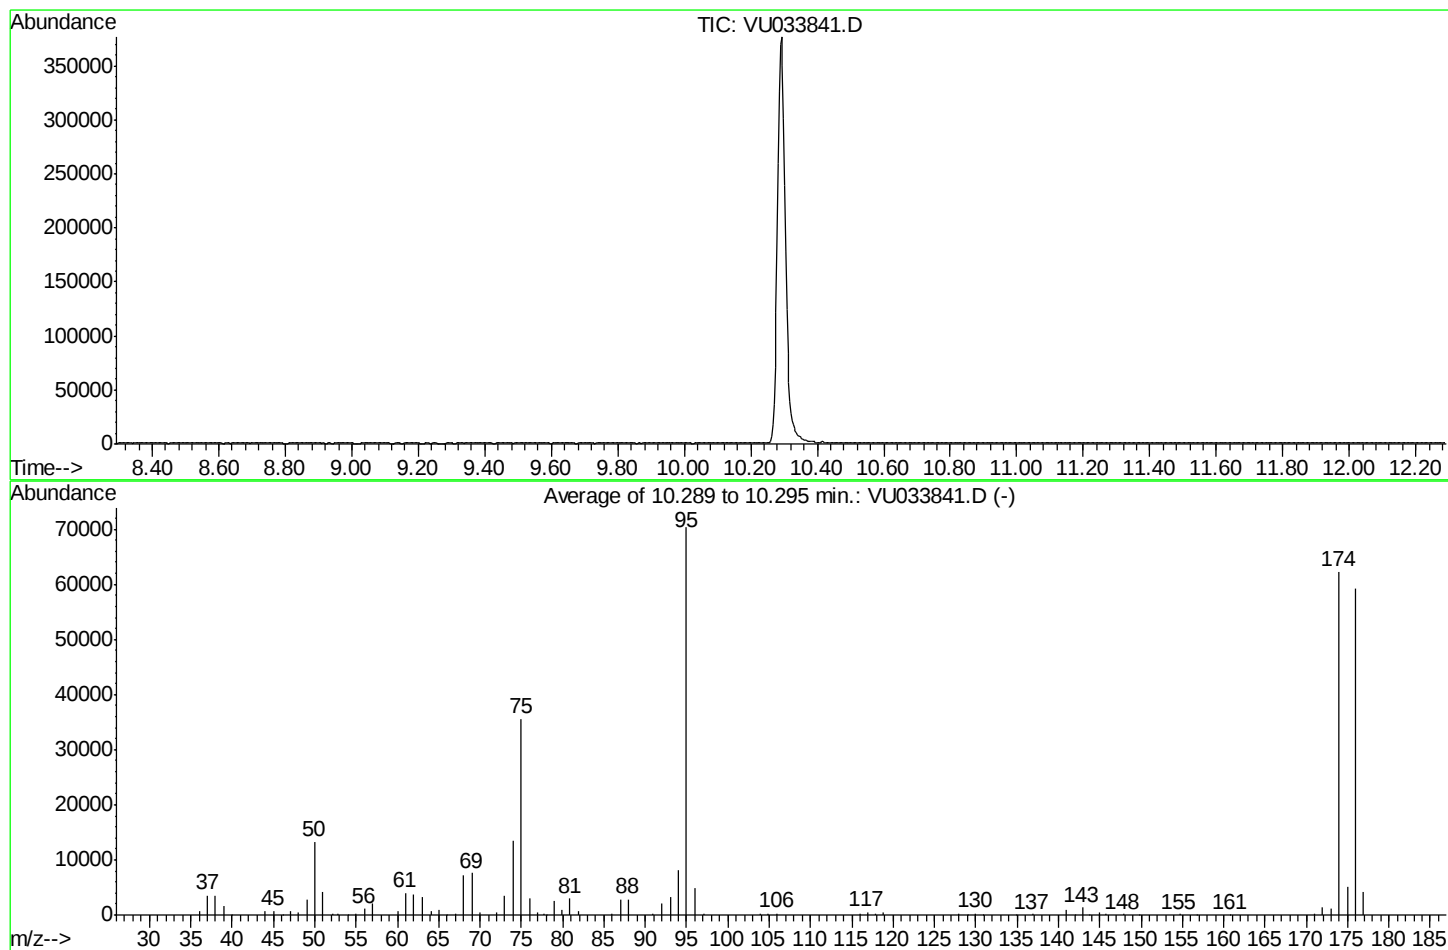

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	13361	PASS
75	95	30	80	50.5	35544	PASS
95	95	100	100	100.0	70336	PASS
96	95	5	9	7.0	4900	PASS
173	174	0.00	2	1.9	1191	PASS
174	95	50	120	88.6	62352	PASS
175	174	5	9	8.1	5020	PASS
176	174	95	101	95.1	59325	PASS
177	176	5	9	7.2	4271	PASS

m/z	Abundance
36.00	744.0
37.00	3601.0
38.00	3500.0
39.00	1537.0
40.10	325.0
44.00	1264.0
45.10	744.0
47.00	702.0
48.00	467.0
49.00	2915.0
50.00	14186.0
51.00	4309.0
52.10	209.0
52.90	104.0
54.90	201.0
56.00	1188.0
57.00	2092.0
60.10	649.0
61.00	3974.0
62.00	3733.0
63.00	3386.0
64.00	658.0
65.00	877.0
67.00	248.0
68.00	7264.0
69.00	7853.0
70.00	487.0
72.10	497.0
73.00	3265.0
74.00	14134.0
75.00	36160.0
76.00	3125.0
77.00	394.0
77.80	309.0
78.90	2769.0
80.00	909.0
80.90	3059.0
81.90	634.0
86.00	237.0
87.00	2656.0
87.90	2942.0
90.80	305.0
92.00	2186.0
93.00	3088.0
94.00	8502.0
95.00	70616.0
96.00	5034.0
97.10	136.0
103.90	312.0
104.80	138.0
106.00	332.0
115.90	317.0
116.90	498.0
117.90	288.0
118.90	506.0
127.80	265.0
130.00	252.0
130.80	110.0
134.90	121.0
136.90	183.0
140.90	946.0
142.00	114.0
142.90	1405.0
144.90	522.0
145.80	151.0
147.80	266.0
149.80	112.0
154.60	152.0
156.80	114.0
171.00	218.0
171.80	1312.0
173.00	1229.0
174.00	62480.0
175.00	4959.0
175.90	59376.0
176.90	4271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	853.0
37.00	3579.0
38.00	3627.0
39.00	1648.0
40.00	336.0
44.00	1235.0
45.10	765.0
47.00	654.0
47.90	498.0
49.00	2967.0
50.00	13787.0
51.00	4272.0
52.10	222.0
52.80	171.0
54.00	144.0
55.00	181.0
56.00	1177.0
57.00	2266.0
60.00	724.0
61.00	4219.0
62.00	3700.0
63.00	3320.0
64.00	647.0
65.00	896.0
67.00	237.0
68.00	7482.0
69.00	7919.0
70.00	599.0
72.10	467.0
73.00	3576.0
74.00	13970.0
75.00	36592.0
76.00	3068.0
76.90	393.0
77.80	353.0
78.90	2749.0
79.90	886.0
80.90	3098.0
81.90	662.0
86.00	253.0
87.00	2949.0
87.90	3017.0
90.90	312.0
92.00	2053.0
93.00	3272.0
94.00	8365.0
95.00	72184.0
96.00	4982.0
97.10	142.0
103.90	277.0
104.90	152.0
106.00	307.0
116.00	378.0
116.90	527.0
117.90	298.0
118.90	499.0
127.80	263.0
129.00	138.0
130.00	259.0
130.80	105.0
134.90	115.0
136.90	188.0
140.90	965.0
142.10	113.0
142.90	1306.0
143.80	104.0
144.90	509.0
145.80	211.0
147.90	234.0
149.80	116.0
154.70	160.0
160.80	105.0
171.10	228.0
171.90	1357.0
173.00	1227.0
174.00	64296.0
175.00	5236.0
176.00	61184.0
177.00	4409.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	841.0
37.00	3285.0
38.00	3288.0
39.00	1590.0
40.00	333.0
43.90	1154.0
45.00	709.0
46.10	120.0
47.00	636.0
47.90	502.0
49.00	2730.0
50.00	12110.0
51.00	3989.0
52.20	253.0
52.90	209.0
54.00	148.0
55.10	168.0
56.00	1106.0
57.00	2138.0
60.00	767.0
61.00	3862.0
62.00	3408.0
63.00	3112.0
64.10	604.0
65.00	839.0
65.90	128.0
67.00	191.0
68.00	6823.0
69.00	7172.0
70.00	610.0
72.00	431.0
73.00	3396.0
74.00	12493.0
75.00	33880.0
76.00	2764.0
77.00	397.0
78.10	284.0
78.90	2490.0
79.90	758.0
80.90	2854.0
81.90	620.0
85.90	176.0
87.00	2955.0
87.90	2663.0
90.90	292.0
92.00	1841.0
93.00	3135.0
94.00	7578.0
95.00	68208.0
96.00	4685.0
97.00	102.0
103.80	262.0
104.90	129.0
105.90	316.0
116.00	363.0
116.90	514.0
117.90	294.0
118.80	521.0
127.90	218.0
129.00	128.0
129.90	271.0
130.80	115.0
136.90	131.0
140.90	831.0
142.10	106.0
142.90	1202.0
144.90	414.0
145.80	219.0
147.90	181.0
154.80	145.0
160.80	147.0
171.10	233.0
171.90	1412.0
173.00	1118.0
173.90	60280.0
175.00	4867.0
176.00	57416.0
177.00	4135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Scan 2848 (10.247 min): VU033841.D
BFB04

m/z	Abundance
39.90	286.0
43.90	604.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04