

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044484.D
 Acq On : 20 Aug 2021 13:03
 Operator : SY/MD
 Sample : M3472-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B60

Quant Time: Aug 21 02:48:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 21 02:45:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 8/23/2021 10:54:07 AM

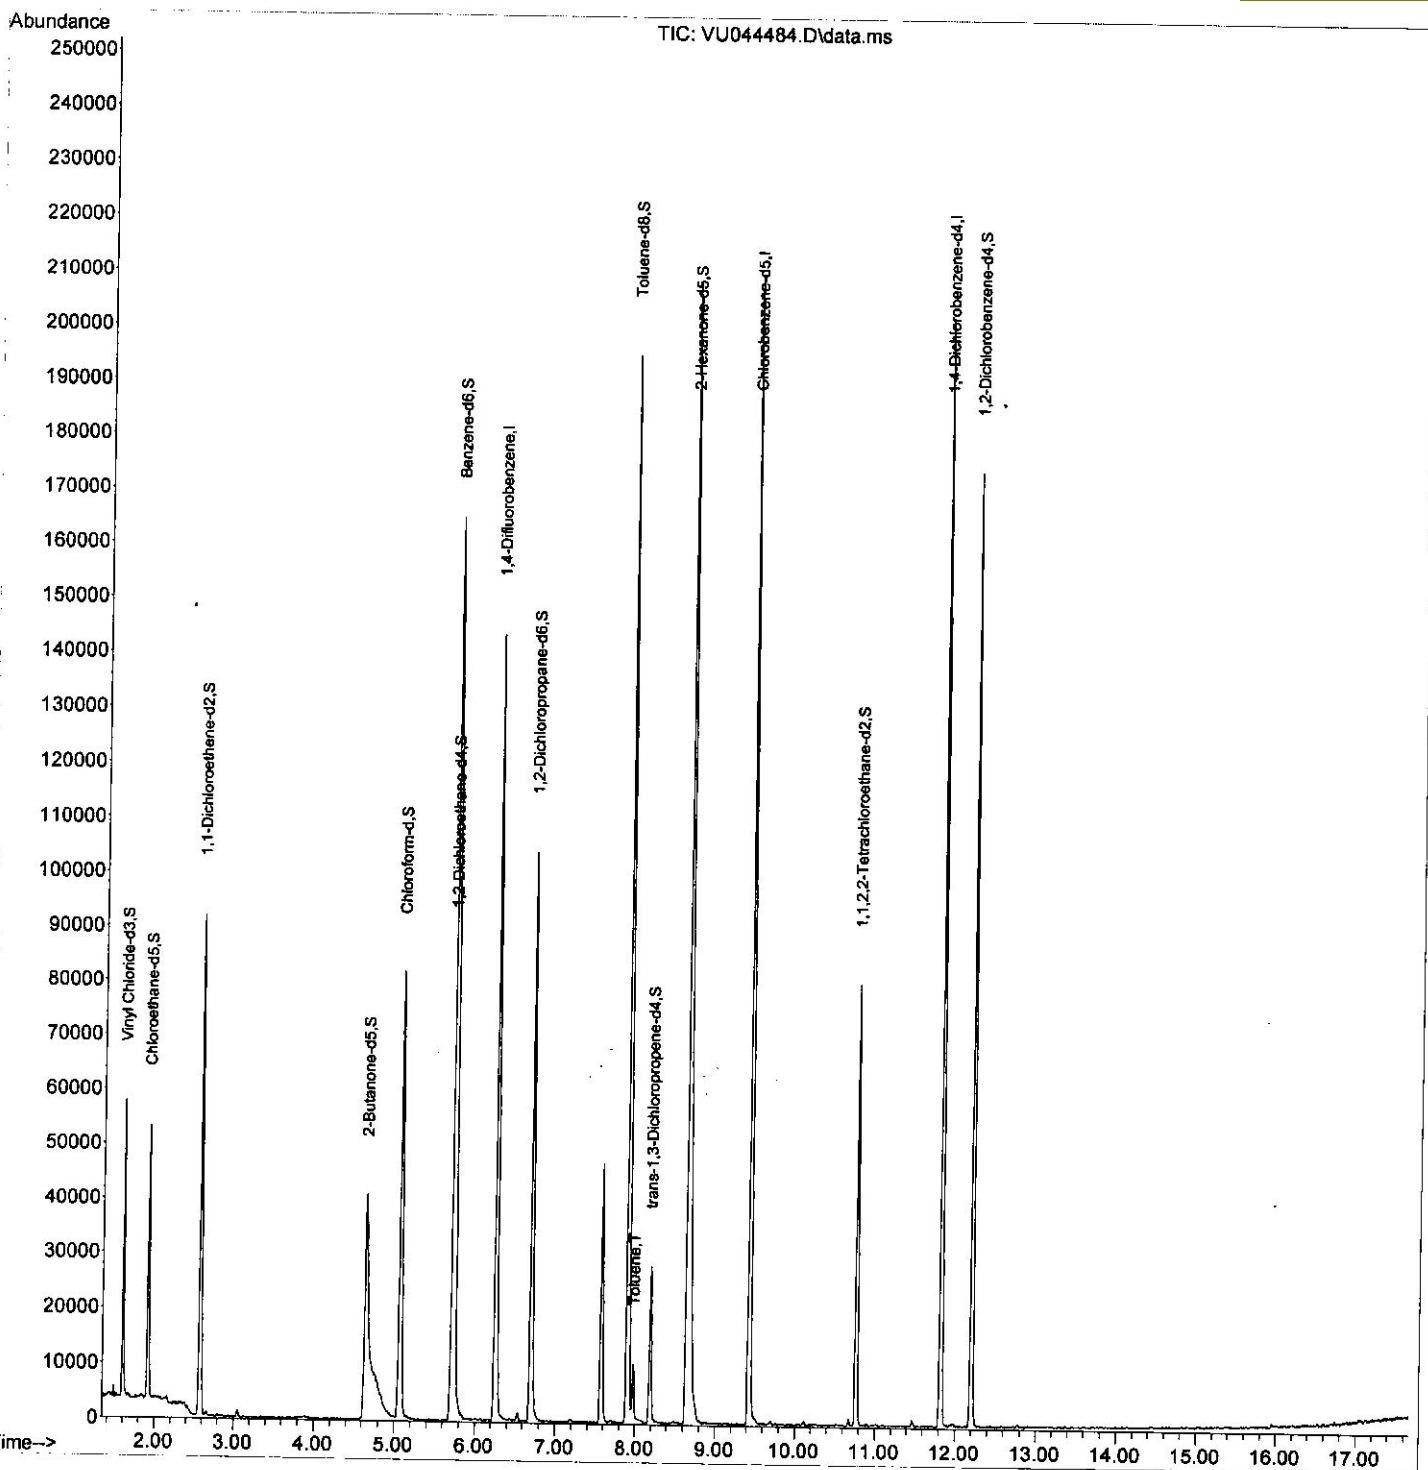

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044484.D
 Acq On : 20 Aug 2021 13:03
 Operator : SY/MD
 Sample : M3472-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B60

Quant Time: Sep 06 03:21:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 03 02:43:14 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 8/23/2021 10:54:07 AM

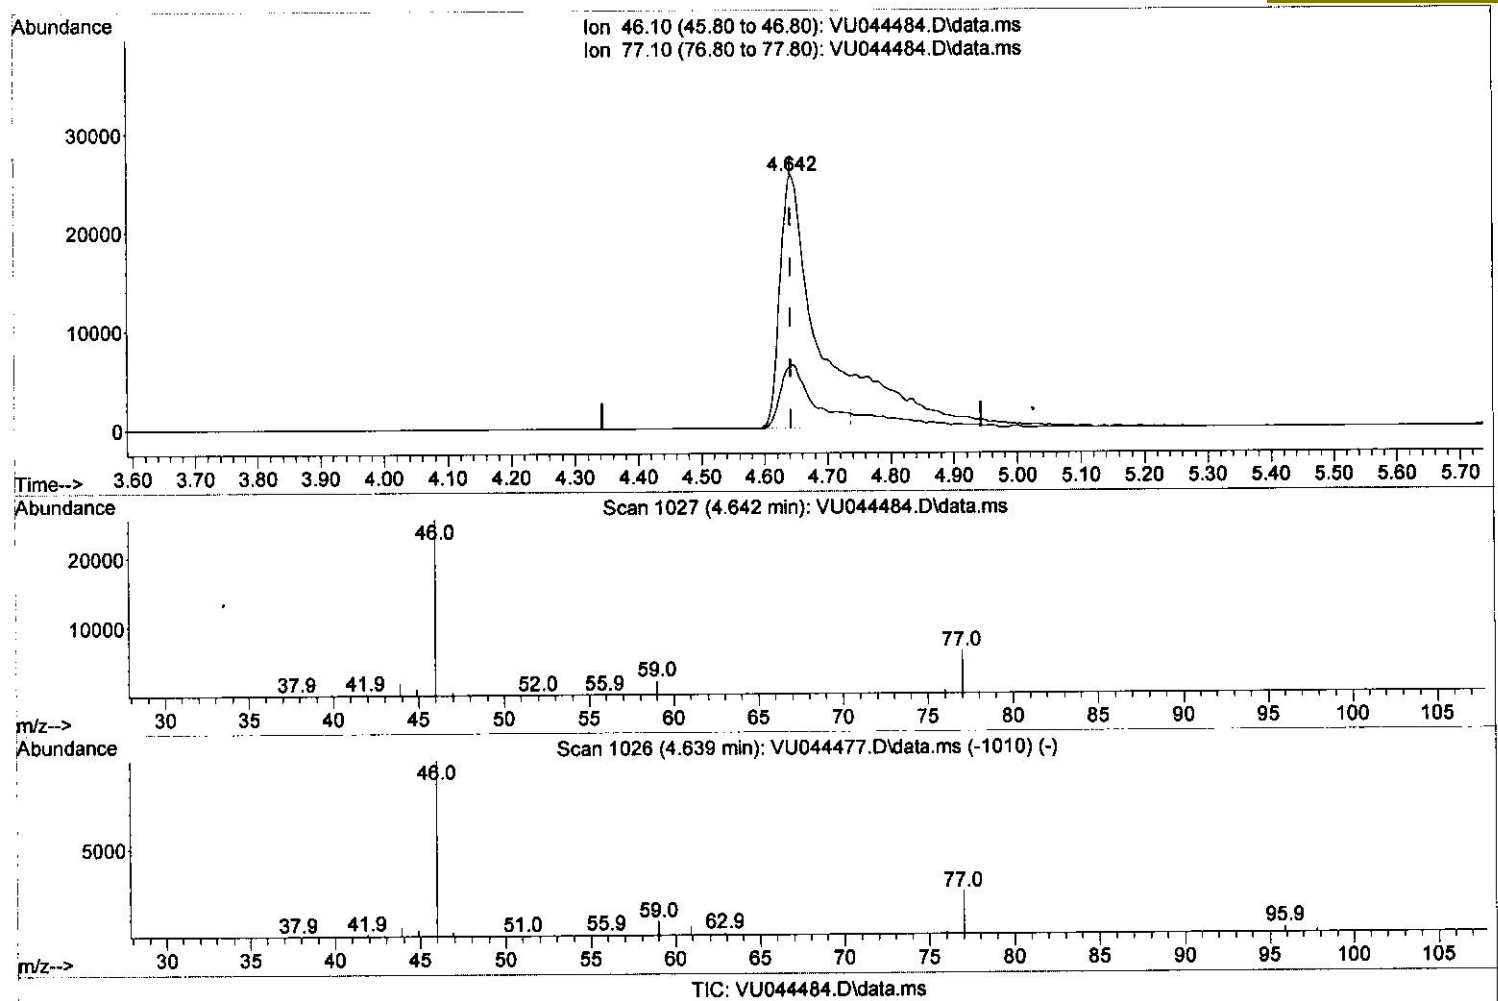

(20) 2-Butanone-d5 (S)

4.642min (+ 0.000) 35.96 ug/L

response 91011

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.00	22.20
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044484.D
 Acq On : 20 Aug 2021 13:03
 Operator : SY/MD
 Sample : M3472-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B60

Quant Time: Aug 21 02:48:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 21 02:45:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 8/23/2021 10:54:07 AM

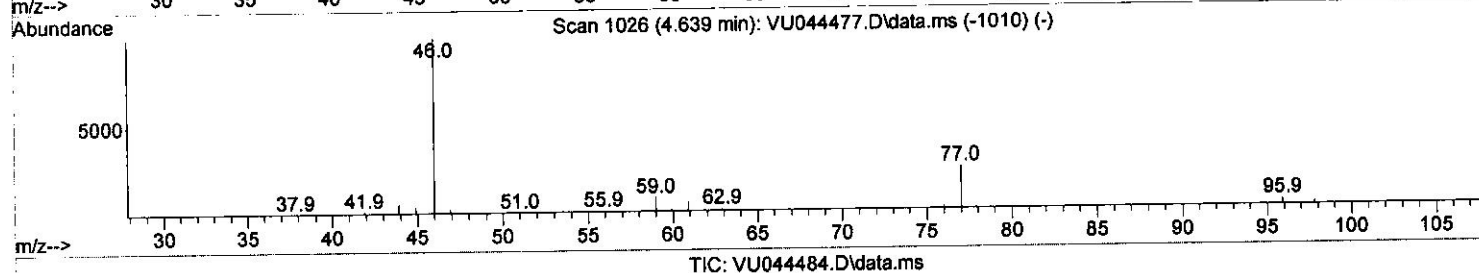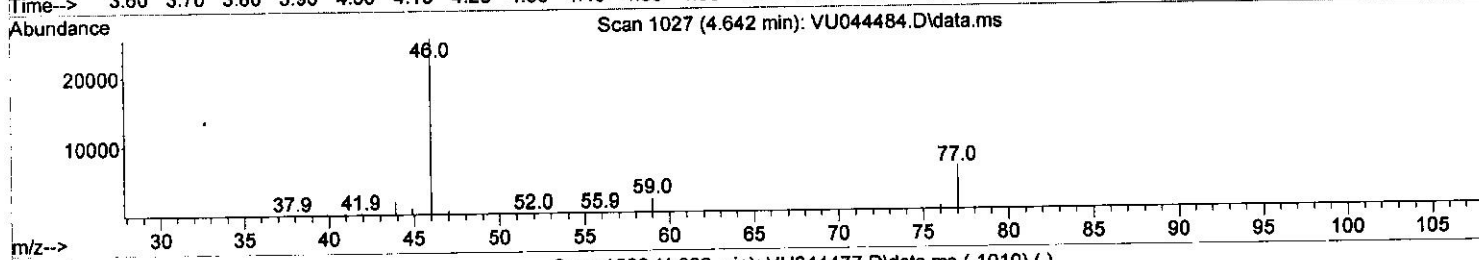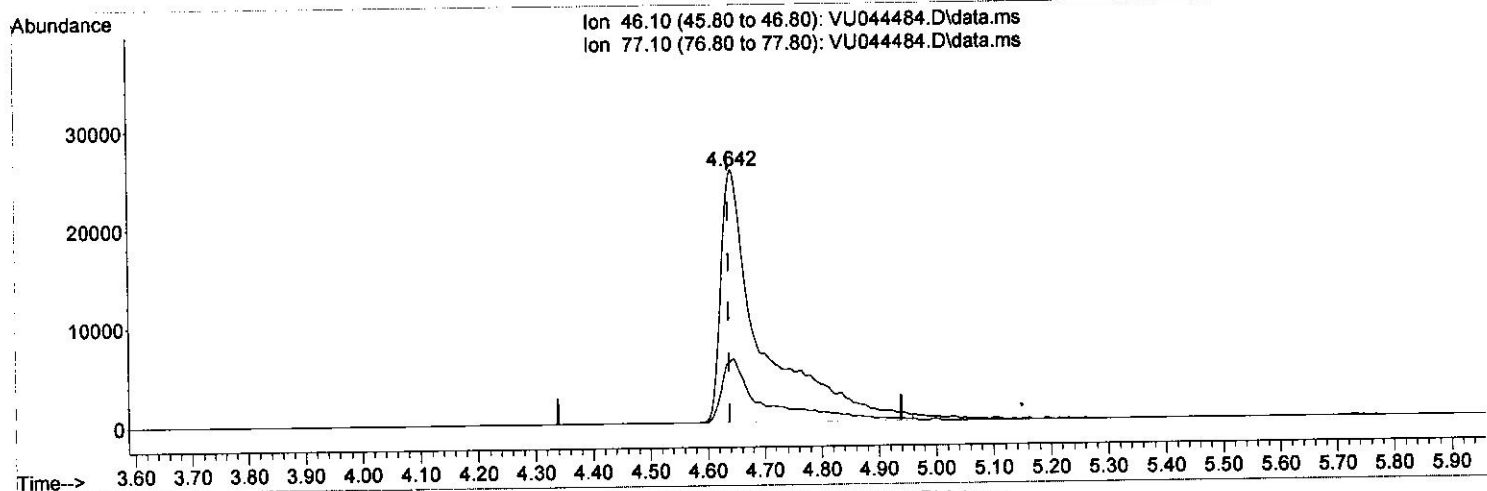

(20) 2-Butanone-d5 (S)

4.642min (+ 0.004) 49.46 ug/L *MD 9/17/21*

response 125190

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.00	16.14#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044484.D
 Acq On : 20 Aug 2021 13:03
 Operator : SY/MD
 Sample : M3472-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B60

Quant Time: Aug 21 02:48:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 21 02:45:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 8/23/2021 10:54:07 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	113150	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.424	117	113535	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	50370	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	37881	4.139	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.800%	
7) Chloroethane-d5	1.916	69	37015	4.654	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.572	65	17830	4.580	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	91.600%	
20) 2-Butanone-d5	4.642	46	125190m	49.465	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.920%	
24) Chloroform-d	5.070	84	75887	4.690	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	5.710	65	42534	4.820	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
32) Benzene-d6	5.736	84	152953	4.784	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.697	67	50423	4.930	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.600%	
41) Toluene-d8	7.903	98	126876	4.475	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.600%	
43) trans-1,3-Dichloroprop...	8.186	79	16185	4.406	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.200%	
46) 2-Hexanone-d5	8.646	63	102870	51.790	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.580%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	41665	4.837	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4	12.198	152	43579	5.121	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.400%	
Target Compounds						
42) Toluene	7.977	91	7460	0.186	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed