

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044484.D
 Acq On : 20 Aug 2021 13:03
 Operator : SY/MD
 Sample : M3472-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B60

Manual Integrations
 APPROVED

SAM
 8/23/2021 10:54:07 AM

Quant Time: Aug 21 02:48:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 21 02:45:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	113150	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.424	117	113535	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	50370	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	37881	4.139	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.800%
7) Chloroethane-d5	1.916	69	37015	4.654	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.572	65	17830	4.580	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.600%
20) 2-Butanone-d5	4.642	46	125190m	49.465	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.920%
24) Chloroform-d	5.070	84	75887	4.690	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	5.710	65	42534	4.820	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.400%
32) Benzene-d6	5.736	84	152953	4.784	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	6.697	67	50423	4.930	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.903	98	126876	4.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	8.186	79	16185	4.406	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.646	63	102870	51.790	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.580%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	41665	4.837	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	43579	5.121	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds					Qvalue	
42) Toluene	7.977	91	7460	0.186	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
Data File : VU044484.D
Acq On : 20 Aug 2021 13:03
Operator : SY/MD
Sample : M3472-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0B60

Manual Integrations
APPROVED


SAM
8/23/2021 10:54:07 AM

Quant Time: Aug 21 02:48:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 21 02:45:30 2021
Response via : Initial Calibration


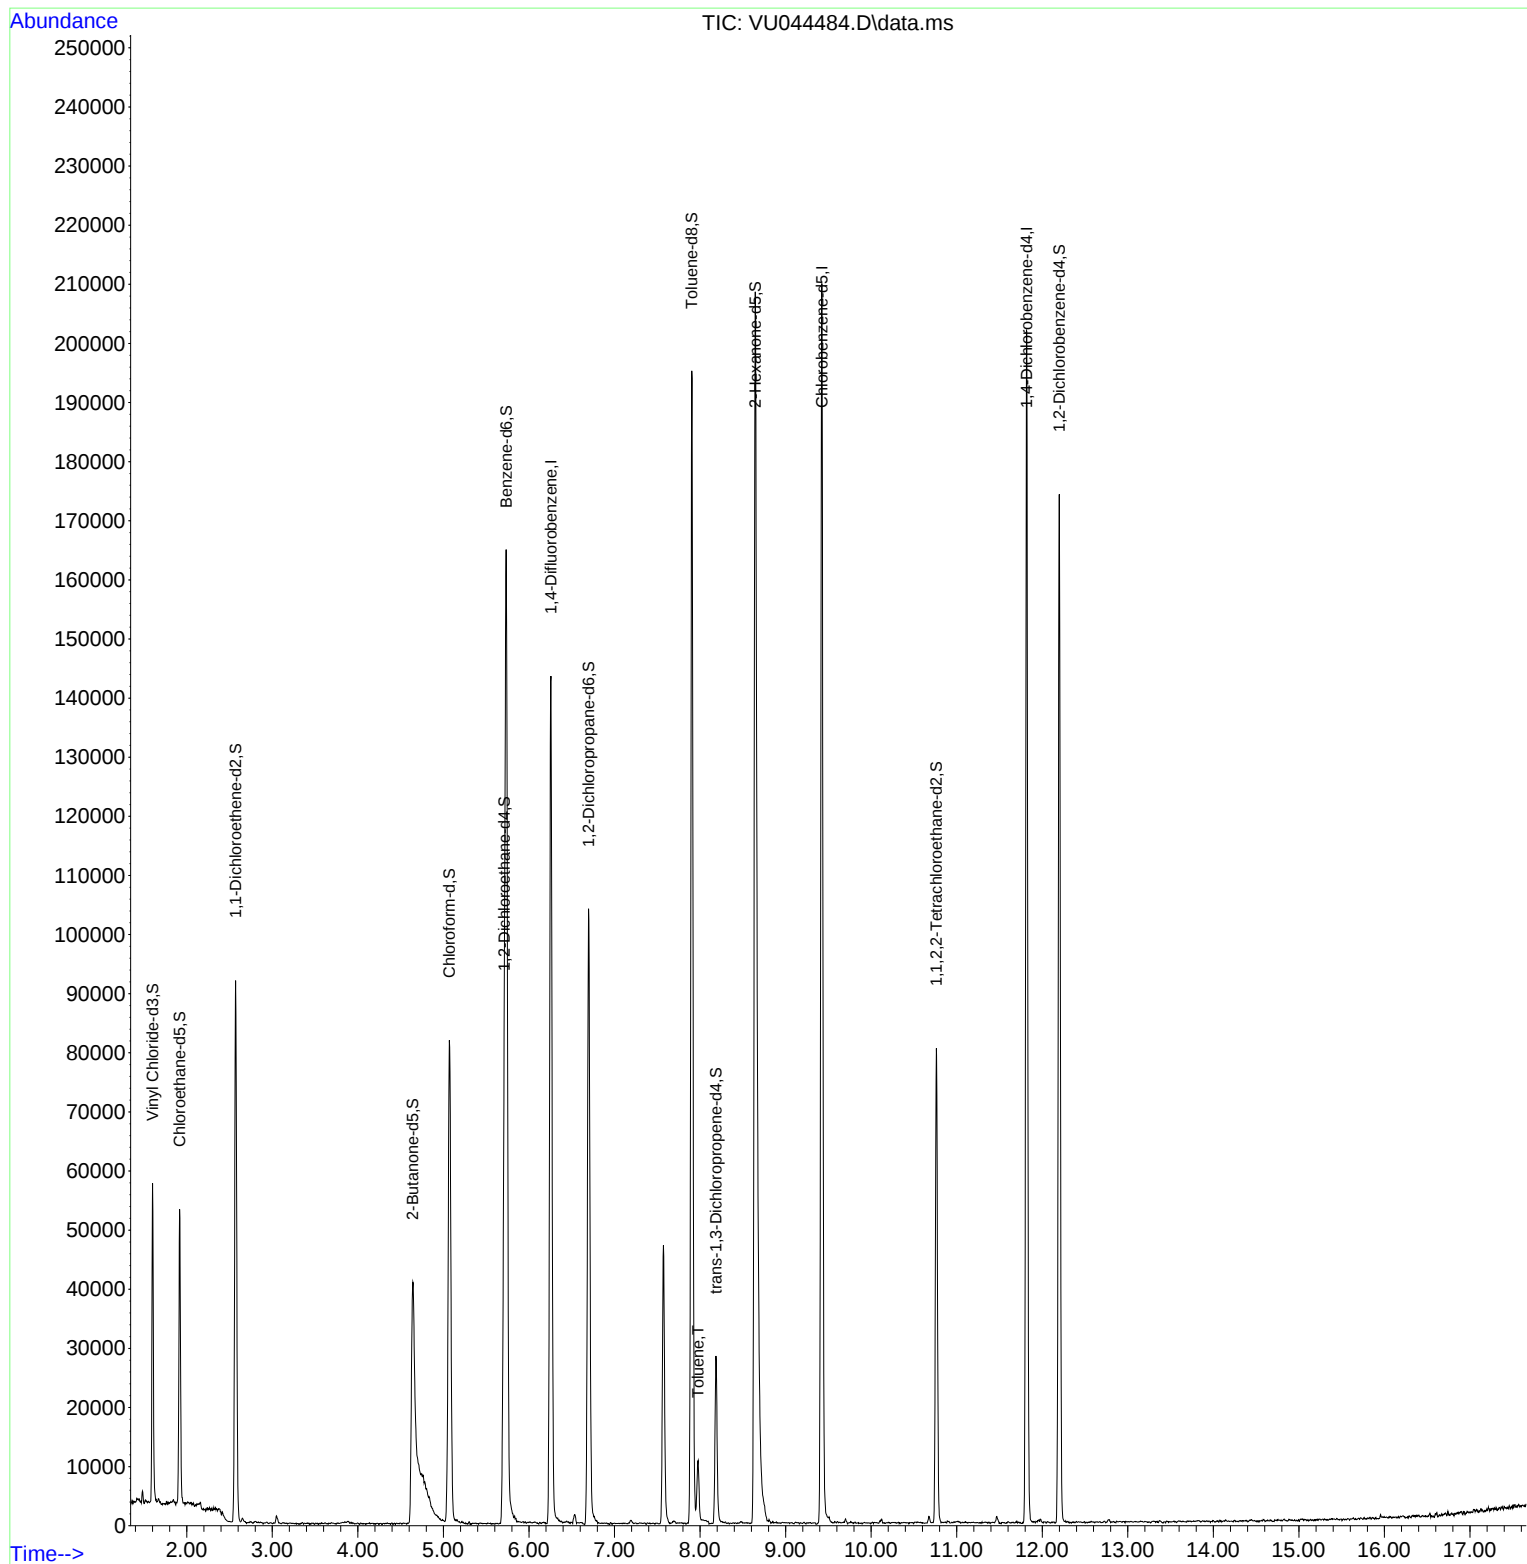


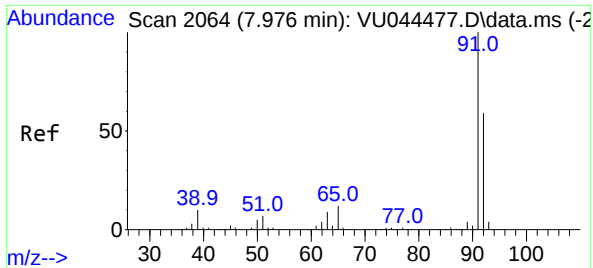

#42
Toluene
Concen: 0.186 ug/L
RT: 7.977 min Scan# 2064
Delta R.T. 0.000 min
Lab File: VU044484.D
Acq: 20 Aug 2021 13:03

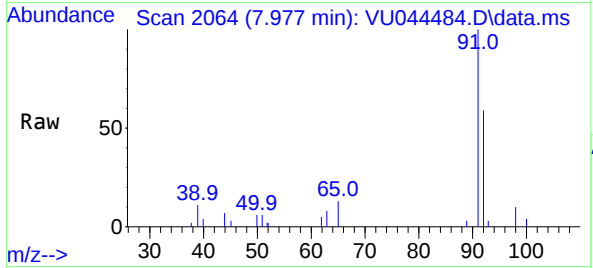

Tgt Ion: 91 Resp: 7460
Ion Ratio Lower Upper
91 100
92 59.4 40.7 75.5

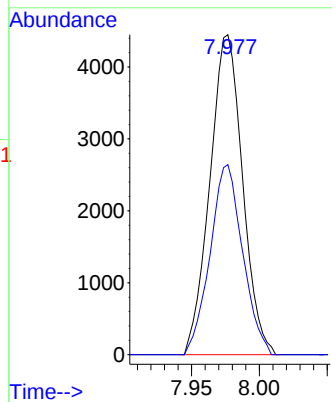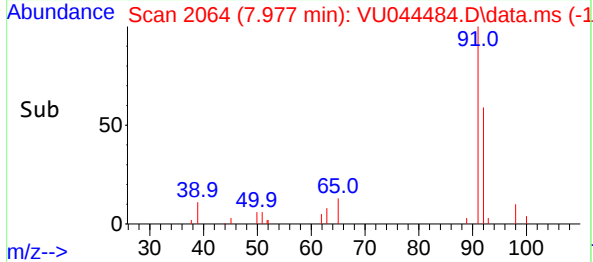

Instrument :
MSVOA_U
ClientSampleId :
C0B60

Manual Integrations
APPROVED

SAM
8/23/2021 10:54:07 AM