

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044483.D
 Acq On : 20 Aug 2021 12:39
 Operator : SY/MD
 Sample : M3472-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	94	rBV	56556	63549	12.11%	1.683%
2	1.915	171	179	198	rVB	50190	66399	12.65%	1.759%
3	2.571	371	383	401	rBV	92114	149674	28.52%	3.964%
4	4.642	1013	1027	1053	rBV	42809	147847	28.18%	3.916%
5	5.070	1143	1160	1181	rBV	92053	208610	39.75%	5.525%
6	5.732	1344	1366	1398	rBV2	167191	437794	83.43%	11.595%
7	6.256	1513	1529	1551	rBV	146307	280844	53.52%	7.438%
8	6.697	1652	1666	1687	rBV	104673	206754	39.40%	5.476%
9	7.571	1927	1938	1964	rBV	46525	84414	16.09%	2.236%
10	7.906	2028	2042	2056	rBV	199653	344517	65.65%	9.124%
11	7.976	2056	2064	2076	rVB	9305	16184	3.08%	0.429%
12	8.185	2119	2129	2148	rBV	28860	49683	9.47%	1.316%
13	8.645	2255	2272	2312	rBV	218005	524742	100.00%	13.898%
14	9.423	2499	2514	2550	rBV	220007	368324	70.19%	9.755%
15	9.574	2550	2561	2572	rBV	7034	11060	2.11%	0.293%
16	9.700	2588	2600	2615	rVB	26084	43467	8.28%	1.151%
17	10.105	2714	2726	2744	rVB	10274	16244	3.10%	0.430%
18	10.764	2919	2931	2948	rBV	79124	129923	24.76%	3.441%
19	11.819	3243	3259	3280	rBV	210884	337648	64.35%	8.942%
20	12.198	3364	3377	3392	rBV	176194	288122	54.91%	7.631%


Sum of corrected areas: 3775799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
Data File : VU044483.D
Acq On : 20 Aug 2021 12:39
Operator : SY/MD
Sample : M3472-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

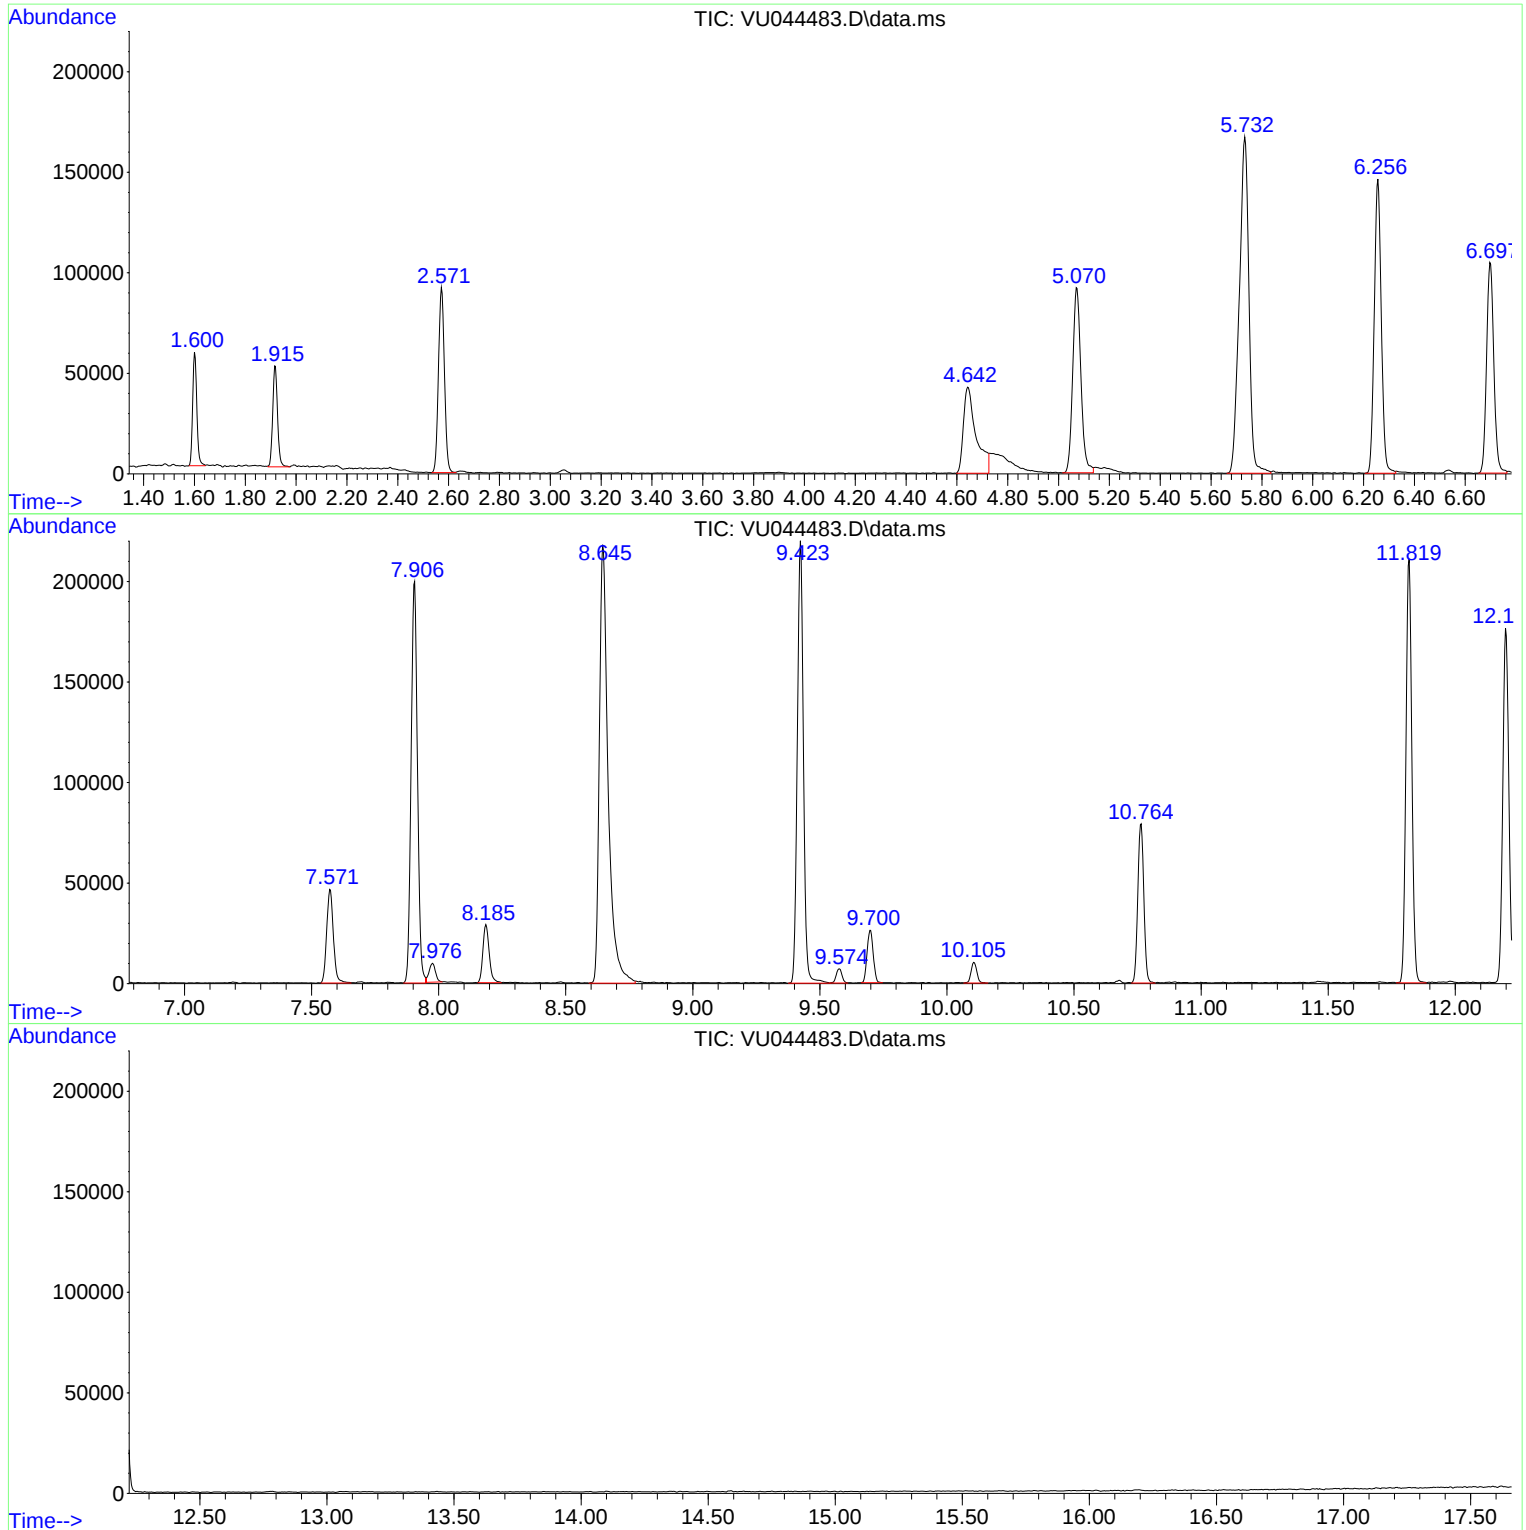

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
Data File : VU044483.D
Acq On : 20 Aug 2021 12:39
Operator : SY/MD
Sample : M3472-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
Data File : VU044483.D
Acq On : 20 Aug 2021 12:39
Operator : SY/MD
Sample : M3472-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
