


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082021\
 Data File : VU044476.D
 Acq On : 20 Aug 2021 09:02
 Operator : SY/MD
 Sample : BFB008
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB008

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 21 02:45:30 2021

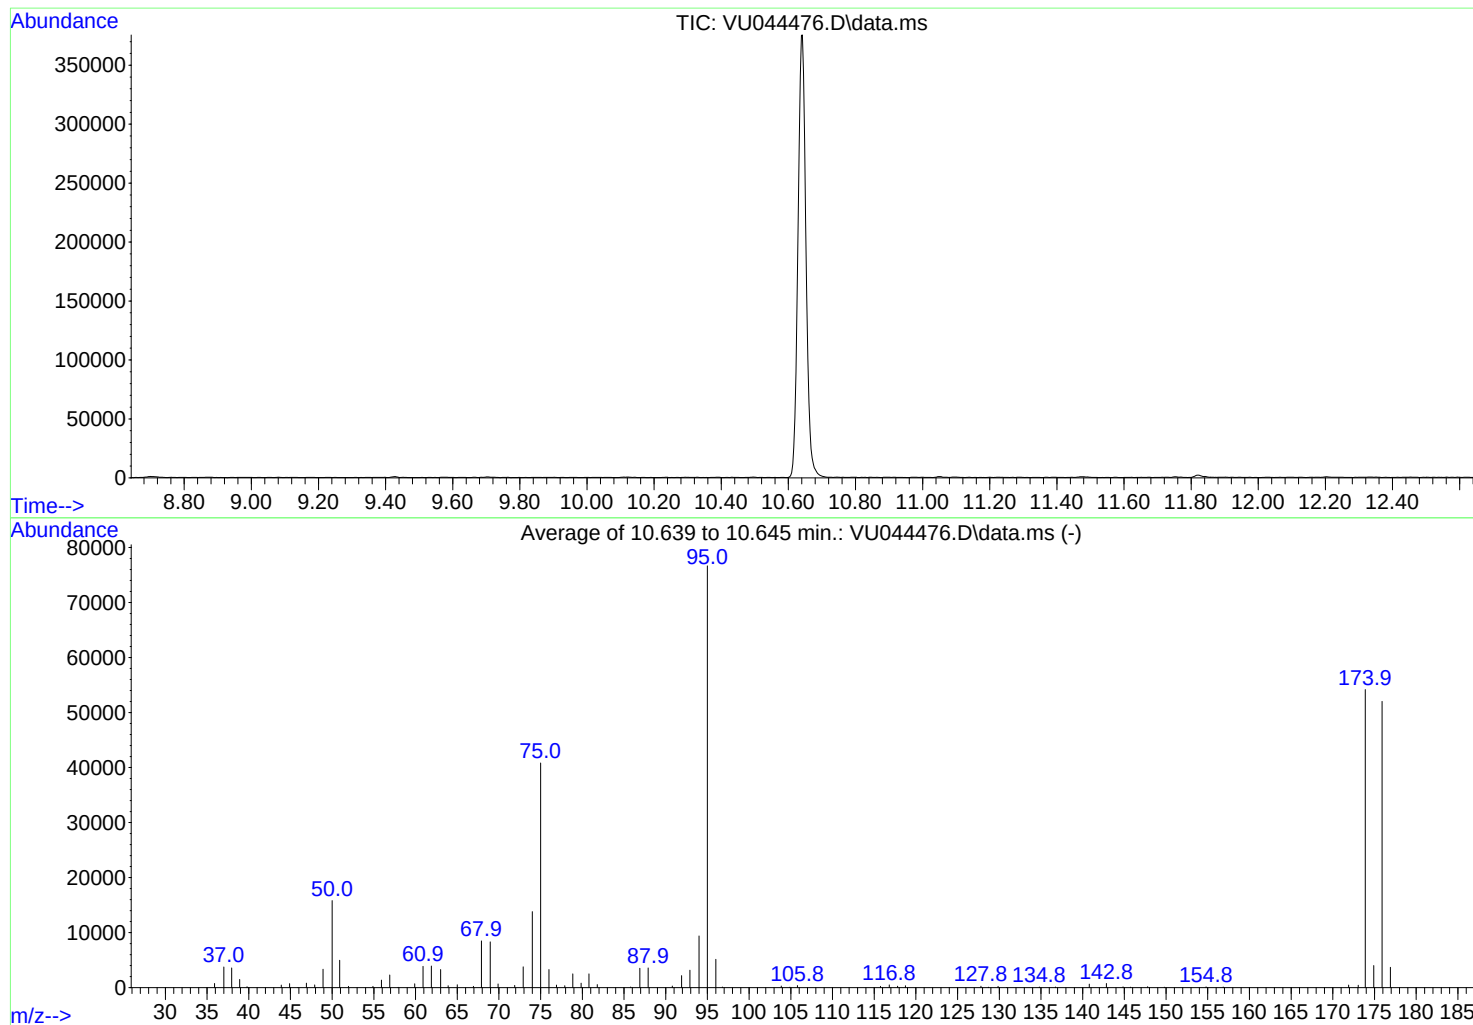

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	15808	PASS
75	95	30	80	53.2	40816	PASS
95	95	100	100	100.0	76661	PASS
96	95	5	9	6.7	5154	PASS
173	174	0.00	2	0.8	446	PASS
174	95	50	120	70.7	54165	PASS
175	174	5	9	7.4	4009	PASS
176	174	95	101	96.1	52029	PASS
177	176	5	9	7.1	3698	PASS

m/z	Abundance
35.90	679.0
37.00	3563.0
37.90	3259.0
38.90	1378.0
39.80	161.0
43.90	758.0
44.90	651.0
46.90	831.0
47.90	457.0
48.90	3061.0
50.00	14393.0
50.90	4535.0
52.00	237.0
54.90	221.0
55.90	1253.0
56.90	2111.0
57.90	117.0
59.90	628.0
60.90	3634.0
61.90	3665.0
63.00	3105.0
63.90	307.0
65.00	397.0
66.90	225.0
67.90	7973.0
69.00	7681.0
69.90	609.0
71.90	412.0
72.90	3603.0
74.00	12829.0
75.00	38040.0
76.00	3084.0
76.90	395.0
77.90	338.0
78.90	2314.0
79.80	780.0
80.80	2394.0
81.80	500.0
85.80	100.0
86.90	3217.0
87.90	3379.0
90.80	227.0
91.90	2025.0
92.90	2936.0
94.00	8762.0
95.00	72080.0
96.00	4779.0
96.80	111.0
103.90	231.0
104.90	127.0
105.80	354.0
115.80	236.0
116.80	484.0
117.80	245.0
118.80	354.0
127.80	247.0
128.70	108.0
129.90	230.0
134.70	128.0
136.80	111.0
140.80	556.0
142.90	723.0
144.80	139.0
145.70	125.0
147.80	150.0
154.80	138.0
156.80	104.0
171.90	424.0
173.00	638.0
173.90	51872.0
174.90	3743.0
175.90	50240.0
176.90	3442.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
43.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	810.0
37.00	3859.0
37.90	3780.0
38.90	1569.0
39.80	201.0
43.90	781.0
44.90	780.0
45.90	110.0
46.90	828.0
47.90	541.0
48.90	3511.0
50.00	16712.0
50.90	5296.0
51.90	214.0
54.90	251.0
55.90	1403.0
56.90	2439.0
59.90	754.0
60.90	4050.0
61.90	4084.0
63.00	3369.0
63.90	416.0
65.00	618.0
67.00	217.0
67.90	8765.0
68.90	8680.0
69.90	687.0
71.90	418.0
72.90	3792.0
74.00	14356.0
75.00	42376.0
76.00	3402.0
76.90	563.0
77.90	368.0
78.80	2618.0
79.90	840.0
80.80	2552.0
81.80	576.0
85.80	119.0
86.90	3711.0
87.90	3646.0
90.80	329.0
91.90	2298.0
92.90	3366.0
94.00	9811.0
95.00	78864.0
96.00	5416.0
96.80	123.0
103.80	324.0
105.80	379.0
115.70	265.0
116.80	485.0
117.80	313.0
118.80	347.0
127.80	278.0
129.80	229.0
134.90	138.0
136.70	124.0
140.80	676.0
142.80	787.0
144.90	129.0
147.80	193.0
149.80	122.0
154.80	185.0
156.90	147.0
171.90	481.0
173.10	699.0
173.90	54792.0
174.90	4133.0
175.90	52024.0
176.90	3790.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	774.0
37.00	3835.0
38.00	3699.0
38.90	1510.0
39.80	184.0
43.90	802.0
44.90	740.0
46.90	831.0
47.90	536.0
48.90	3442.0
50.00	16319.0
50.90	5118.0
52.00	240.0
54.90	249.0
55.90	1423.0
56.90	2375.0
57.90	100.0
59.90	716.0
60.90	3943.0
61.90	4067.0
63.00	3367.0
63.90	367.0
65.00	532.0
66.90	223.0
67.90	8715.0
69.00	8567.0
69.90	678.0
71.90	427.0
72.90	3939.0
74.00	14255.0
75.00	42032.0
76.00	3417.0
76.90	484.0
77.90	370.0
78.90	2564.0
79.90	852.0
80.80	2586.0
81.80	560.0
85.80	124.0
86.90	3630.0
87.90	3690.0
90.80	298.0
91.90	2221.0
92.90	3239.0
94.00	9604.0
95.00	79040.0
96.00	5268.0
96.80	130.0
103.80	288.0
104.90	111.0
105.80	402.0
115.70	251.0
116.80	518.0
117.80	277.0
118.70	331.0
127.80	259.0
128.70	123.0
129.90	223.0
130.90	106.0
134.80	117.0
136.70	115.0
140.80	661.0
142.90	767.0
144.90	134.0
145.80	109.0
147.80	170.0
149.80	112.0
154.80	165.0
156.80	129.0
171.90	480.0
173.90	55832.0
174.90	4152.0
175.90	53824.0
176.90	3862.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008