


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082024\
Data File : VU060484.D
Acq On : 20 Aug 2024 11:43
Operator : MD/SY
Sample : BFB187
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB187

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Aug 21 02:30:39 2024

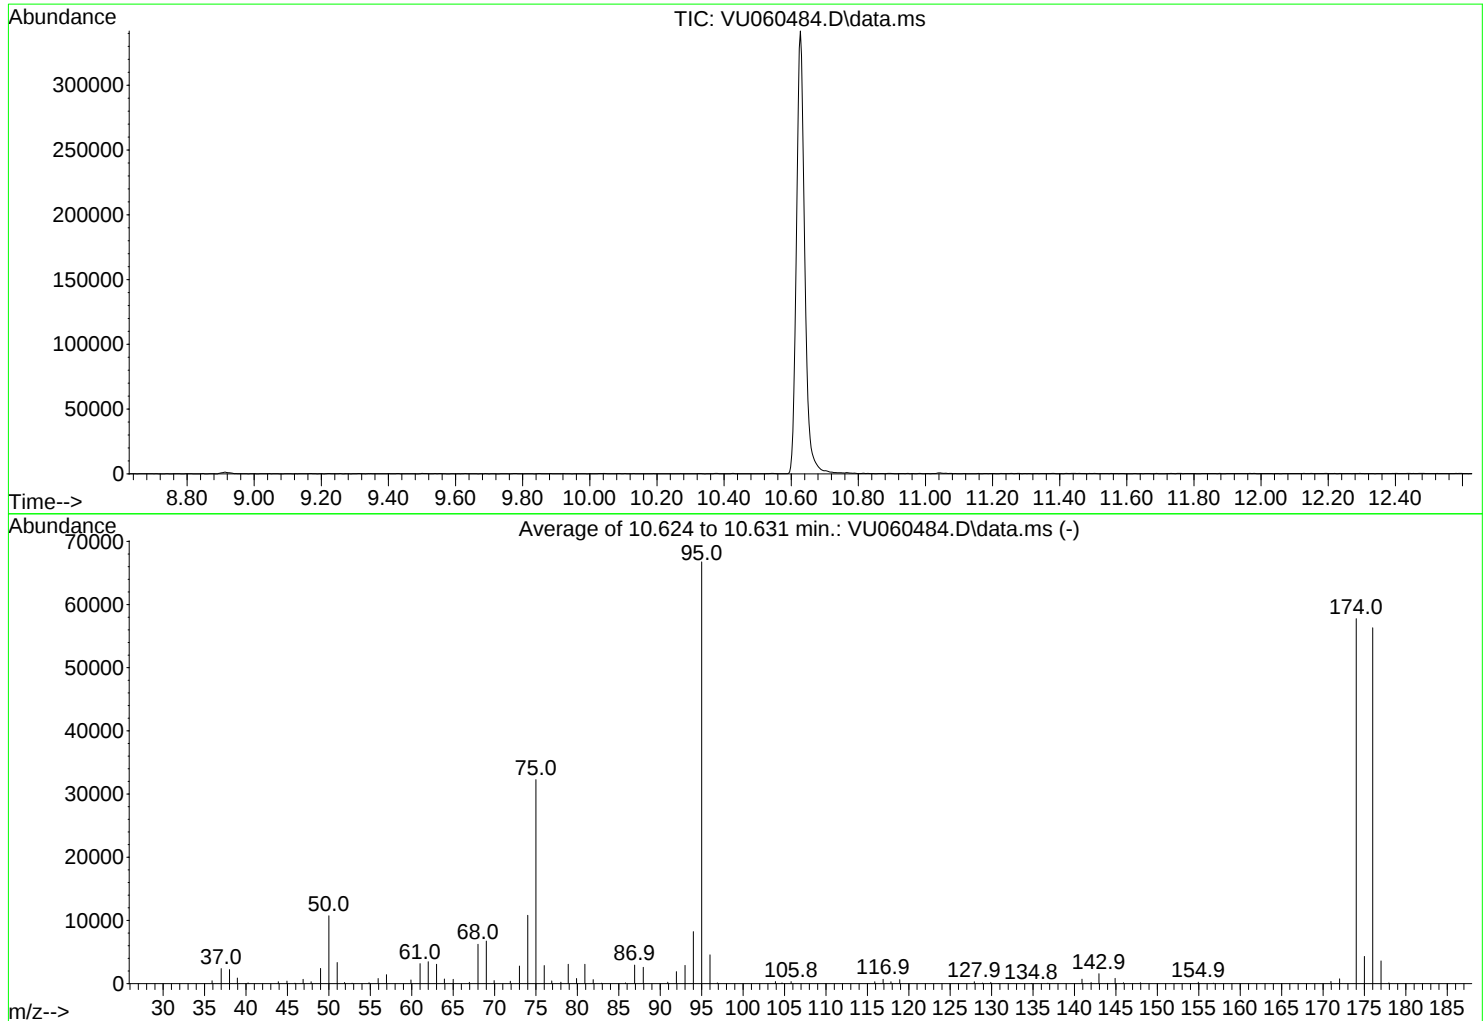

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	10745	PASS
75	95	30	80	48.4	32283	PASS
95	95	100	100	100.0	66755	PASS
96	95	5	9	6.8	4551	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.5	57771	PASS
175	174	5	9	7.5	4313	PASS
176	174	95	101	97.5	56317	PASS
177	176	5	9	6.4	3608	PASS

m/z	Abundance
43.90	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
35.90	445.0
37.00	2397.0
38.00	2322.0
38.90	1014.0
40.30	116.0
43.90	513.0
44.90	410.0
46.90	775.0
47.90	359.0
49.00	2356.0
50.00	10525.0
51.00	3192.0
51.90	189.0
52.80	140.0
54.80	157.0
56.00	826.0
56.90	1430.0
59.90	621.0
61.00	3334.0
62.00	3523.0
63.00	3033.0
63.90	761.0
65.00	746.0
66.90	176.0
68.00	6299.0
69.00	6672.0
70.00	480.0
71.90	392.0
73.00	2884.0
74.00	10852.0
75.00	32584.0
76.00	2890.0
76.90	408.0
78.00	266.0
78.90	3113.0
79.90	789.0
80.90	3013.0
81.90	608.0
85.70	140.0
86.90	3142.0
88.00	2697.0
90.90	221.0
92.00	2073.0
93.00	2924.0
94.00	8036.0
95.00	66112.0
96.00	4700.0
96.90	122.0
103.90	323.0
104.70	125.0
105.80	348.0
115.90	235.0
116.90	617.0
117.80	280.0
118.90	650.0
127.90	271.0
129.90	222.0
136.80	138.0
140.90	704.0
142.00	168.0
143.00	1626.0
144.00	127.0
144.90	865.0
145.90	120.0
147.90	122.0
155.00	249.0
156.80	128.0
170.90	363.0
172.00	713.0
174.00	56624.0
175.00	4261.0
176.00	54560.0
177.00	3781.0
178.00	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
35.90	462.0
37.00	2486.0
38.00	2357.0
39.00	928.0
40.20	121.0
43.90	486.0
44.90	413.0
45.90	101.0
46.90	720.0
47.90	314.0
49.00	2525.0
50.00	11144.0
51.00	3507.0
51.90	190.0
52.80	117.0
54.80	154.0
55.90	834.0
56.90	1464.0
59.90	603.0
61.00	3232.0
62.00	3625.0
63.00	3167.0
63.90	766.0
65.00	718.0
66.90	205.0
68.00	6347.0
69.00	6958.0
70.00	510.0
71.90	393.0
73.00	2911.0
74.00	11177.0
75.00	33192.0
76.00	2978.0
76.90	445.0
78.00	237.0
78.90	3156.0
79.90	833.0
80.90	3195.0
81.90	679.0
82.90	104.0
85.80	132.0
86.90	3008.0
87.90	2723.0
90.90	229.0
92.00	1896.0
93.00	2955.0
94.00	8591.0
95.00	69000.0
96.00	4655.0
96.90	128.0
103.90	330.0
104.70	128.0
105.80	345.0
115.90	300.0
116.90	732.0
117.80	312.0
118.90	635.0
127.90	335.0
128.90	134.0
129.90	222.0
130.80	104.0
136.80	105.0
140.90	711.0
142.00	208.0
143.00	1630.0
144.90	894.0
145.90	156.0
148.00	154.0
155.00	250.0
156.80	125.0
171.00	386.0
172.00	750.0
174.00	59520.0
175.00	4469.0
176.00	58008.0
177.00	3711.0
177.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
35.90	466.0
37.00	2249.0
38.00	2050.0
39.00	728.0
40.20	122.0
43.90	417.0
45.00	367.0
45.90	107.0
46.90	581.0
47.80	243.0
49.00	2364.0
50.00	10565.0
51.00	3324.0
51.90	191.0
54.90	154.0
56.00	782.0
57.00	1382.0
59.90	506.0
61.00	2949.0
62.00	3269.0
63.00	3009.0
64.00	682.0
65.00	623.0
67.00	201.0
68.00	6065.0
69.00	6543.0
69.90	490.0
71.90	347.0
73.00	2581.0
74.00	10405.0
75.00	31072.0
76.00	2739.0
76.90	464.0
78.00	204.0
78.90	2927.0
79.90	787.0
80.90	2994.0
81.90	639.0
82.90	109.0
85.90	104.0
86.90	2662.0
87.90	2347.0
90.90	232.0
91.90	1707.0
93.00	2777.0
94.00	8070.0
95.00	65152.0
96.00	4299.0
96.90	108.0
103.90	313.0
104.70	104.0
105.80	312.0
115.90	353.0
116.90	742.0
117.90	284.0
118.90	602.0
127.90	302.0
128.90	170.0
129.90	210.0
134.80	126.0
140.90	699.0
142.00	186.0
142.90	1452.0
144.90	768.0
145.90	162.0
147.90	168.0
154.90	207.0
171.00	350.0
172.00	812.0
174.00	57168.0
175.00	4210.0
176.00	56384.0
177.00	3331.0
177.90	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187