


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082118\
Data File : VU026220.D
Acq On : 21 Aug 2018 09:47
Operator : MD/SY
Sample : BFB41
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 22 00:24:50 2018

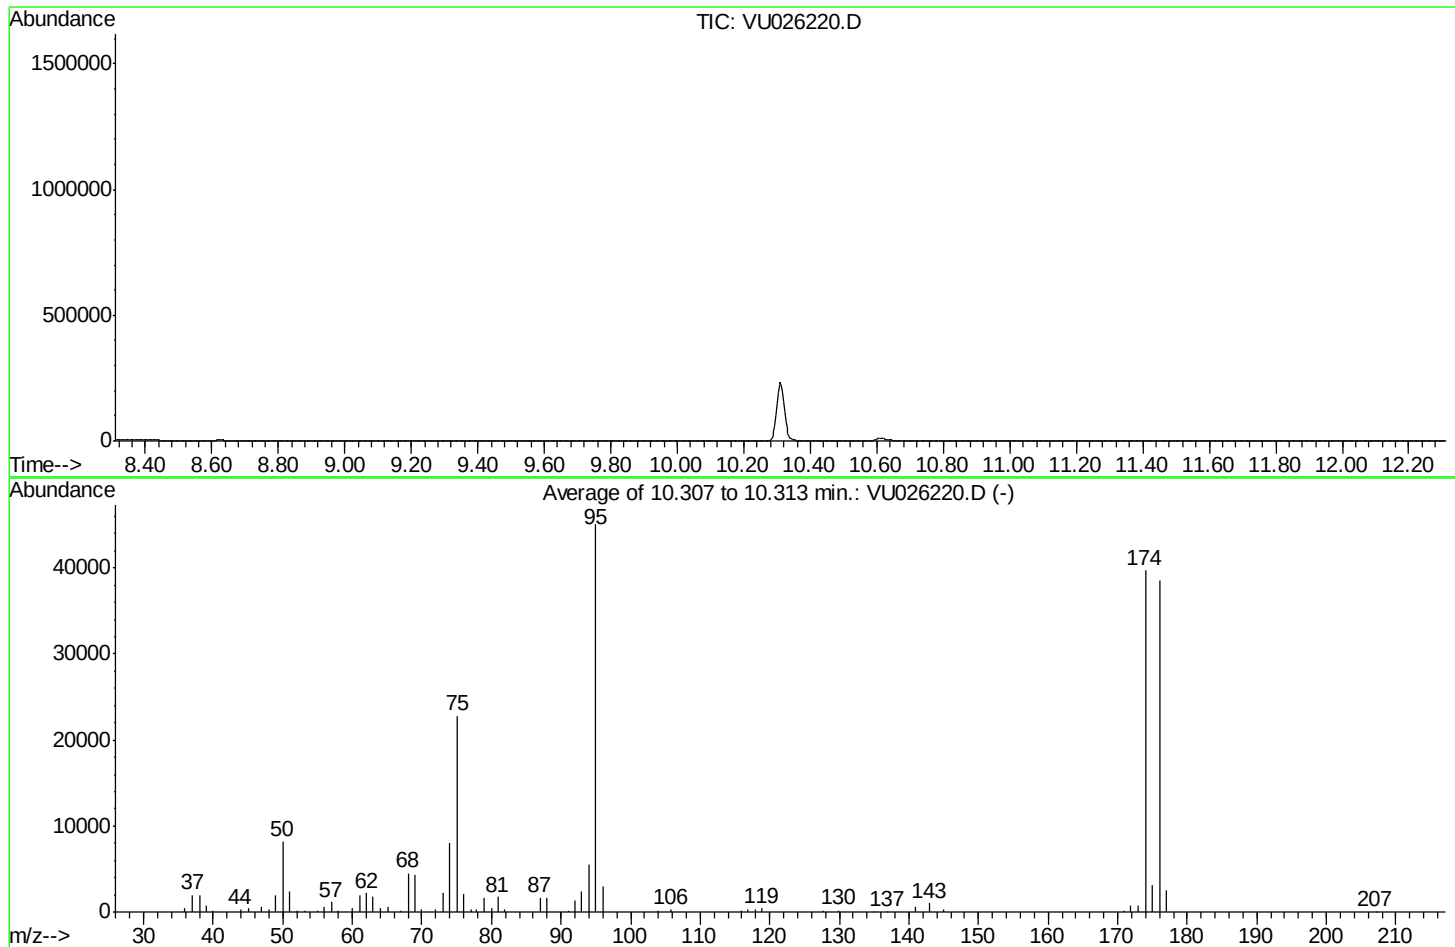

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3009

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8136	PASS
75	95	30	80	50.7	22840	PASS
95	95	100	100	100.0	45066	PASS
96	95	5	9	6.7	3000	PASS
173	174	0.00	2	1.7	692	PASS
174	95	50	120	88.1	39712	PASS
175	174	5	9	7.8	3090	PASS
176	174	95	101	96.9	38472	PASS
177	176	5	9	6.5	2497	PASS

Scan 3009 (10.265 min): VU026220.D
BFB41

m/z	Abundance
39.90	124.0
43.90	391.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	436.0
37.00	2167.0
38.00	1945.0
39.00	817.0
40.00	212.0
44.00	676.0
45.10	422.0
47.00	647.0
48.00	304.0
49.00	1970.0
50.00	8032.0
51.00	2333.0
52.10	161.0
53.10	109.0
55.10	189.0
56.00	631.0
57.00	1032.0
60.00	341.0
61.00	1894.0
62.10	2268.0
63.00	1648.0
64.00	411.0
65.10	527.0
66.90	148.0
68.00	4559.0
69.00	4477.0
69.90	311.0
72.00	328.0
73.00	2333.0
74.00	8310.0
75.10	22776.0
76.00	2175.0
77.00	282.0
77.90	195.0
78.90	1656.0
79.90	468.0
80.90	1642.0
82.00	315.0
86.90	1711.0
87.90	1483.0
91.00	206.0
92.00	1311.0
93.00	2342.0
94.00	5544.0
95.00	43984.0
96.00	3045.0
103.90	173.0
105.80	286.0
116.00	256.0
116.90	397.0
117.90	280.0
118.90	379.0
127.70	144.0
130.00	139.0
134.90	108.0
140.90	602.0
143.00	939.0
145.00	235.0
170.90	166.0
171.90	746.0
173.00	748.0
174.00	38568.0
174.90	2901.0
176.00	36672.0
176.90	2390.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	463.0
37.00	2038.0
38.00	2046.0
39.00	819.0
40.00	254.0
44.00	646.0
45.10	416.0
47.00	655.0
48.00	287.0
49.00	2015.0
50.00	8485.0
51.00	2480.0
52.10	124.0
53.10	143.0
55.10	145.0
56.00	680.0
57.00	1184.0
57.90	107.0
60.00	385.0
61.00	2046.0
62.00	2236.0
63.00	1760.0
64.00	414.0
65.10	617.0
67.00	102.0
68.00	4648.0
69.00	4398.0
69.90	367.0
72.00	324.0
73.00	2306.0
74.00	8330.0
75.10	23536.0
76.00	2237.0
77.10	264.0
77.90	279.0
78.90	1639.0
80.00	471.0
80.90	1812.0
82.00	325.0
87.00	1700.0
87.90	1635.0
91.00	199.0
92.00	1324.0
93.00	2538.0
94.00	5764.0
95.00	46664.0
96.00	3115.0
103.90	222.0
105.90	291.0
116.00	188.0
116.90	350.0
117.90	270.0
118.90	413.0
127.70	162.0
130.00	182.0
141.00	533.0
143.00	1115.0
145.00	265.0
170.90	190.0
171.90	771.0
172.90	742.0
174.00	40848.0
174.90	3205.0
176.00	39680.0
177.00	2583.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	435.0
37.00	1769.0
38.00	1959.0
39.00	744.0
40.00	232.0
44.00	571.0
45.10	338.0
47.00	587.0
47.90	275.0
49.00	1927.0
50.00	7891.0
51.00	2453.0
53.10	159.0
54.90	113.0
56.00	652.0
57.00	1171.0
57.90	136.0
60.00	420.0
61.00	2038.0
62.00	2146.0
63.00	1760.0
64.00	373.0
65.10	629.0
68.00	4232.0
69.00	3948.0
69.90	373.0
72.00	234.0
73.00	2044.0
74.00	7627.0
75.10	22208.0
76.00	1940.0
77.10	239.0
77.90	330.0
78.90	1620.0
80.00	469.0
80.90	1815.0
81.80	296.0
87.00	1677.0
87.90	1591.0
91.00	181.0
92.00	1259.0
93.00	2480.0
94.00	5419.0
95.00	44552.0
96.00	2841.0
103.90	248.0
105.90	216.0
115.90	157.0
116.90	317.0
117.90	257.0
118.90	355.0
127.70	155.0
129.90	174.0
136.90	112.0
140.90	513.0
143.00	1042.0
145.00	272.0
170.80	188.0
171.90	742.0
172.90	586.0
174.00	39720.0
174.90	3166.0
176.00	39064.0
177.00	2519.0
207.10	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41