

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033871.D
 Acq On : 21 Aug 2019 14:27
 Operator : JC/SP
 Sample : K4420-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	86	93	108	rBV	259099	270524	16.93%	2.243%
2	1.669	173	180	193	rVB	221015	271955	17.02%	2.255%
3	2.257	353	363	376	rVB	378115	576036	36.06%	4.777%
4	2.595	465	468	470	rBV	452	291	0.02%	0.002%
5	2.679	492	494	495	rBV	414	160	0.01%	0.001%
6	2.904	561	564	567	rVB	308	152	0.01%	0.001%
7	2.929	569	572	576	rVB3	378	296	0.02%	0.002%
8	2.958	576	581	585	rBV3	753	620	0.04%	0.005%
9	2.994	590	592	597	rBV2	237	178	0.01%	0.001%
10	3.016	597	599	601	rBV	256	119	0.01%	0.001%
11	3.058	610	612	613	rBV	216	88	0.01%	0.001%
12	3.084	617	620	625	rBV3	410	434	0.03%	0.004%
13	3.158	640	643	646	rVB3	198	168	0.01%	0.001%
14	3.177	646	649	650	rBV2	156	68	0.00%	0.001%
15	3.241	666	669	671	rVB	224	124	0.01%	0.001%
16	3.257	671	674	677	rBV	498	298	0.02%	0.002%
17	3.277	677	680	682	rBV2	171	123	0.01%	0.001%
18	3.309	688	690	692	rVB2	288	136	0.01%	0.001%
19	3.354	701	704	706	rBV2	473	325	0.02%	0.003%
20	3.386	712	714	715	rBV	187	81	0.01%	0.001%
21	3.460	736	737	738	rBV	203	48	0.00%	0.000%
22	3.508	751	752	755	rBV2	127	69	0.00%	0.001%
23	3.569	769	771	774	rVB	228	123	0.01%	0.001%
24	3.595	774	779	781	rBV	164	109	0.01%	0.001%
25	3.614	782	785	787	rBV	192	123	0.01%	0.001%
26	3.650	793	796	799	rVB2	202	100	0.01%	0.001%
27	3.672	799	803	805	rVB	143	108	0.01%	0.001%
28	3.685	805	807	808	rBV	240	90	0.01%	0.001%
29	3.711	813	815	817	rBV	168	71	0.00%	0.001%
30	3.733	817	822	827	rBV2	297	345	0.02%	0.003%
31	3.781	834	837	840	rBV	310	239	0.01%	0.002%
32	3.839	847	855	858	rBV2	426	443	0.03%	0.004%
33	3.868	862	864	866	rVB	219	74	0.00%	0.001%
34	3.884	866	869	873	rBV2	252	173	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033871.D
 Acq On : 21 Aug 2019 14:27
 Operator : JC/SP
 Sample : K4420-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

35	3.904	873	875	878	rVV	306	117	0.01%	0.001%
36	3.949	887	889	892	rVV2	185	114	0.01%	0.001%
37	3.965	892	894	895	rVB2	218	70	0.00%	0.001%
38	4.006	905	907	909	rVB2	219	91	0.01%	0.001%
39	4.026	909	913	918	rVB2	188	214	0.01%	0.002%
40	4.051	918	921	924	rVB2	210	123	0.01%	0.001%
41	4.068	924	926	927	rBV2	193	92	0.01%	0.001%
42	4.090	931	933	935	rVB	241	118	0.01%	0.001%
43	4.106	935	938	939	rBV	206	107	0.01%	0.001%
44	4.151	939	952	991	rBV	115584	392437	24.56%	3.254%
45	4.621	1080	1098	1130	rBV	275635	657809	41.17%	5.455%
46	4.942	1194	1198	1200	rBV3	602	414	0.03%	0.003%
47	5.010	1216	1219	1220	rBV2	197	114	0.01%	0.001%
48	5.035	1224	1227	1228	rVB	181	77	0.00%	0.001%
49	5.048	1229	1231	1236	rVB3	170	110	0.01%	0.001%
50	5.077	1236	1240	1243	rVB3	432	294	0.02%	0.002%
51	5.100	1243	1247	1251	rBV	372	365	0.02%	0.003%
52	5.135	1253	1258	1262	rVB3	327	296	0.02%	0.002%
53	5.164	1262	1267	1268	rBV	258	167	0.01%	0.001%
54	5.209	1279	1281	1282	rBV	160	64	0.00%	0.001%
55	5.315	1290	1314	1339	rBV2	539173	1597652	100.00%	13.249%
56	5.585	1396	1398	1402	rVB2	906	410	0.03%	0.003%
57	5.865	1471	1485	1511	rBV	463095	926259	57.98%	7.681%
58	6.161	1565	1577	1590	rVB4	10141	19826	1.24%	0.164%
59	6.309	1609	1623	1644	rBV	366524	736239	46.08%	6.106%
60	6.543	1694	1696	1697	rBV	408	128	0.01%	0.001%
61	6.592	1708	1711	1713	rBV2	290	195	0.01%	0.002%
62	6.611	1716	1717	1718	rVV	225	48	0.00%	0.000%
63	6.640	1724	1726	1728	rVB2	381	115	0.01%	0.001%
64	6.653	1728	1730	1732	rBV	260	120	0.01%	0.001%
65	6.807	1775	1778	1780	rBV	145	90	0.01%	0.001%
66	6.820	1780	1782	1785	rBV2	155	91	0.01%	0.001%
67	6.836	1785	1787	1789	rBV	172	98	0.01%	0.001%
68	6.862	1793	1795	1798	rVV	524	306	0.02%	0.003%
69	6.900	1804	1807	1809	rBV2	201	96	0.01%	0.001%
70	6.958	1822	1825	1827	rBV	245	133	0.01%	0.001%
71	7.026	1845	1846	1849	rBV2	159	71	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
Data File : VU033871.D
Acq On : 21 Aug 2019 14:27
Operator : JC/SP
Sample : K4420-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B74

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Title : VOC Analysis

72	7.058	1853	1856	1858	rBV2	260	139	0.01%	0.001%
73	7.074	1859	1861	1864	rBV2	358	177	0.01%	0.001%
74	7.103	1868	1870	1874	rVB2	180	104	0.01%	0.001%
75	7.125	1874	1877	1880	rVB	179	122	0.01%	0.001%
76	7.151	1880	1885	1889	rVB2	278	278	0.02%	0.002%
77	7.209	1889	1903	1926	rBV	181000	334051	20.91%	2.770%
78	7.547	1995	2008	2038	rBV	701261	1234172	77.25%	10.235%
79	7.833	2086	2097	2118	rBV	129704	229142	14.34%	1.900%
80	7.990	2144	2146	2149	rVB2	573	318	0.02%	0.003%
81	8.058	2164	2167	2170	rBV2	367	329	0.02%	0.003%
82	8.100	2178	2180	2187	rBV2	332	250	0.02%	0.002%
83	8.125	2187	2188	2190	rBV	134	44	0.00%	0.000%
84	8.141	2190	2193	2194	rBV	241	124	0.01%	0.001%
85	8.193	2207	2209	2212	rBV2	283	200	0.01%	0.002%
86	8.244	2221	2225	2226	rBV3	302	205	0.01%	0.002%
87	8.296	2230	2241	2274	rBV2	355241	700389	43.84%	5.808%
88	8.611	2336	2339	2344	rVB3	736	537	0.03%	0.004%
89	8.765	2383	2387	2388	rBV	542	344	0.02%	0.003%
90	8.807	2398	2400	2401	rBV	305	103	0.01%	0.001%
91	8.952	2441	2445	2449	rBV2	327	343	0.02%	0.003%
92	9.071	2469	2482	2511	rBV	723406	1205764	75.47%	9.999%
93	9.363	2568	2573	2577	rBV2	617	644	0.04%	0.005%
94	9.710	2678	2681	2682	rBV2	249	129	0.01%	0.001%
95	9.990	2766	2768	2769	rBV2	273	108	0.01%	0.001%
96	10.257	2847	2851	2853	rBV2	312	234	0.01%	0.002%
97	10.415	2888	2900	2922	rBV	501202	817866	51.19%	6.783%
98	11.299	3171	3175	3179	rBV2	571	524	0.03%	0.004%
99	11.466	3215	3227	3246	rBV	619009	999211	62.54%	8.286%
100	11.842	3332	3344	3373	rBV	656560	1073200	67.17%	8.900%


Sum of corrected areas: 12058412

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082119\
Data File : VU033871.D
Acq On : 21 Aug 2019 14:27
Operator : JC/SP
Sample : K4420-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

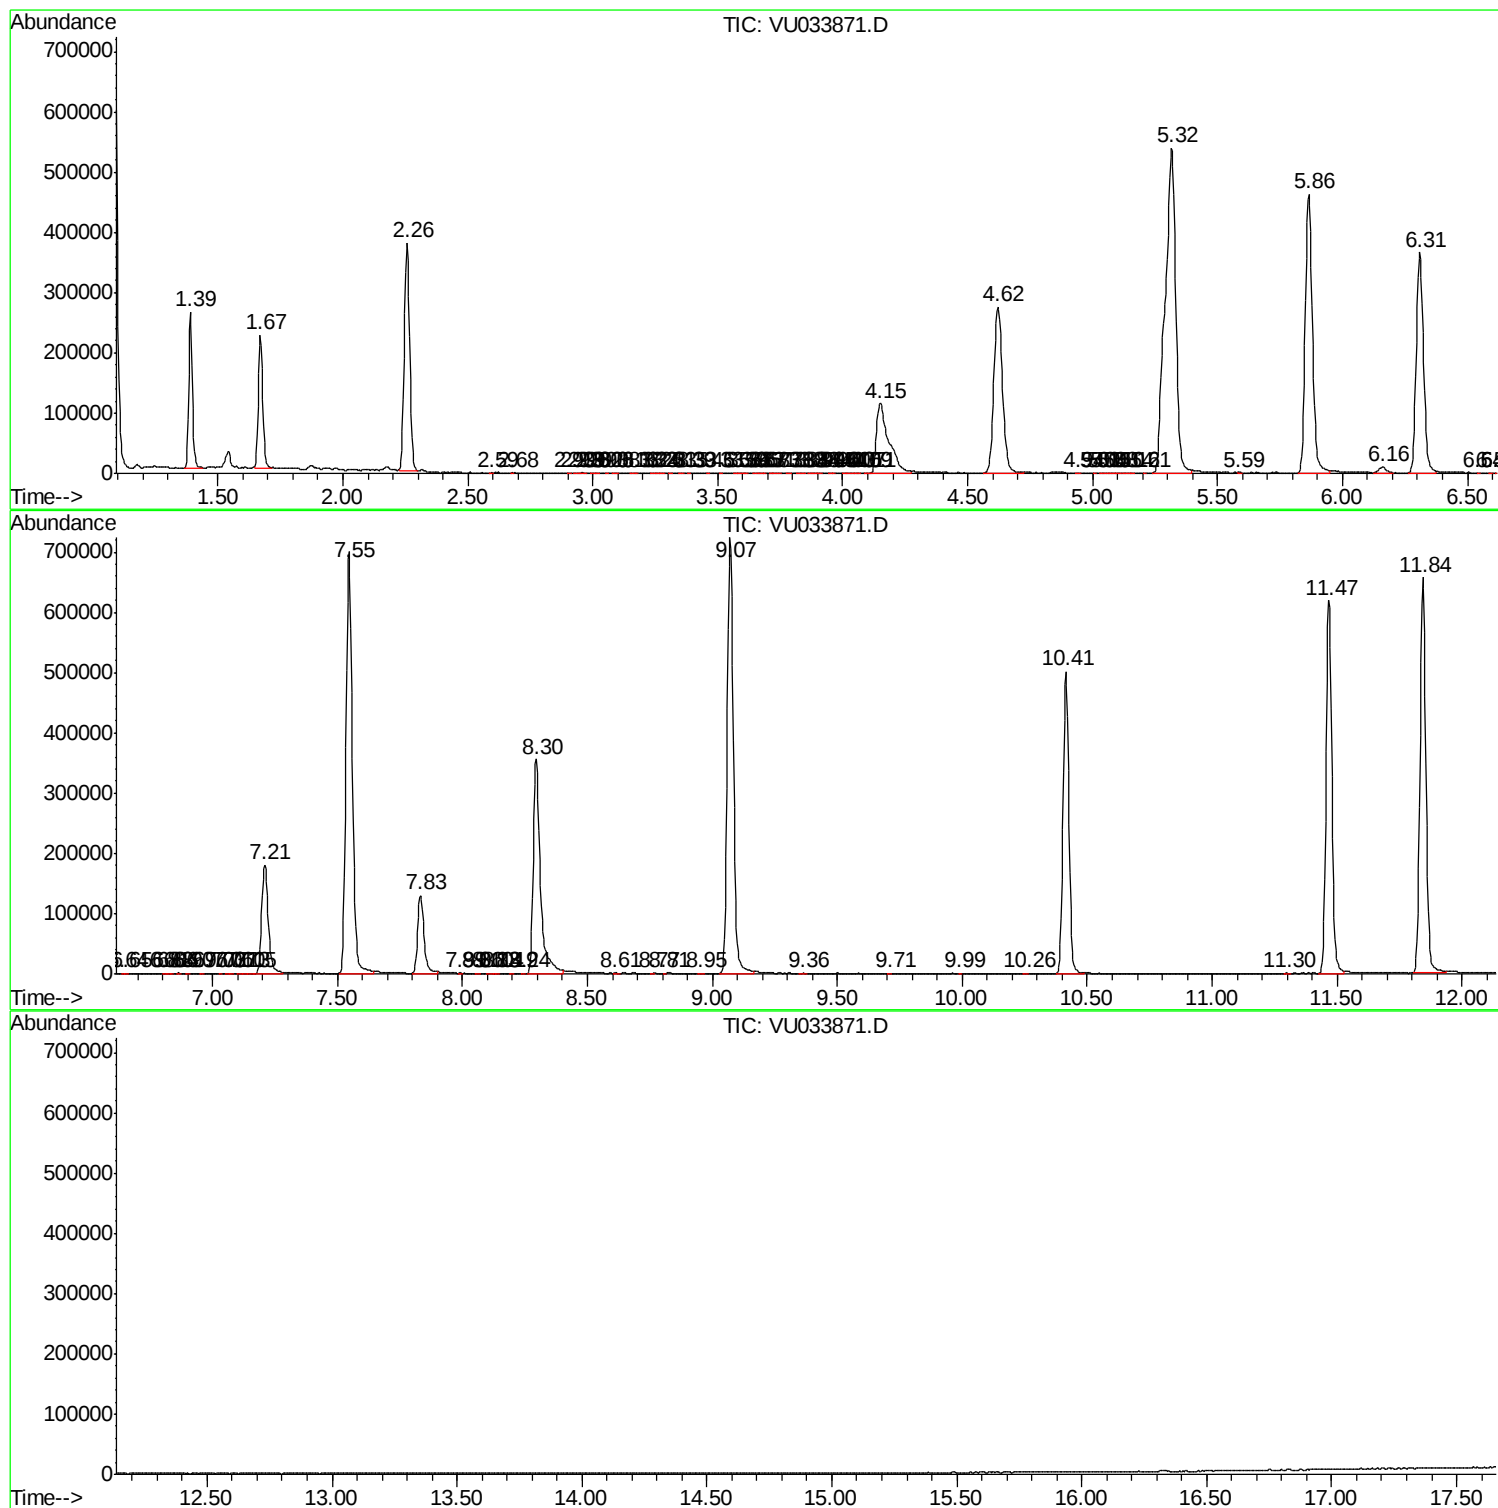

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082119\
Data File : VU033871.D
Acq On : 21 Aug 2019 14:27
Operator : JC/SP
Sample : K4420-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082119\
Data File : VU033871.D
Acq On : 21 Aug 2019 14:27
Operator : JC/SP
Sample : K4420-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc