

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033882.D
 Acq On : 21 Aug 2019 19:21
 Operator : JC/SP
 Sample : K4420-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2C07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	86	93	109	rBV	276583	279287	17.46%	2.320%
2	1.669	173	180	192	rVB	220380	267666	16.73%	2.223%
3	2.254	352	362	377	rVB	387154	592848	37.05%	4.924%
4	2.769	519	522	525	rBV3	438	344	0.02%	0.003%
5	2.827	537	540	542	rBV3	420	254	0.02%	0.002%
6	2.894	560	561	562	rBV3	147	48	0.00%	0.000%
7	2.926	567	571	573	rBV	431	298	0.02%	0.002%
8	2.965	573	583	597	rVV	36627	67248	4.20%	0.559%
9	3.097	621	624	626	rBV	418	256	0.02%	0.002%
10	3.164	642	645	647	rVB2	286	170	0.01%	0.001%
11	3.177	647	649	651	rBV2	298	145	0.01%	0.001%
12	3.241	666	669	671	rBV	326	238	0.01%	0.002%
13	3.254	671	673	676	rVV2	255	160	0.01%	0.001%
14	3.319	691	693	694	rVB2	166	45	0.00%	0.000%
15	3.335	694	698	702	rBV3	649	732	0.05%	0.006%
16	3.422	722	725	731	rVB3	625	474	0.03%	0.004%
17	3.476	739	742	743	rBV	208	124	0.01%	0.001%
18	3.569	768	771	773	rVB2	315	167	0.01%	0.001%
19	3.672	801	803	811	rVB2	432	339	0.02%	0.003%
20	3.762	828	831	832	rBV	258	137	0.01%	0.001%
21	3.814	843	847	849	rBV	233	200	0.01%	0.002%
22	3.881	863	868	872	rBV2	257	266	0.02%	0.002%
23	4.004	903	906	908	rVB	247	108	0.01%	0.001%
24	4.081	929	930	934	rBV2	269	167	0.01%	0.001%
25	4.151	940	952	958	rBV	119773	262628	16.41%	2.181%
26	4.621	1082	1098	1120	rBV	272728	648717	40.55%	5.388%
27	5.048	1229	1231	1236	rBV2	318	225	0.01%	0.002%
28	5.097	1245	1246	1248	rVB2	176	39	0.00%	0.000%
29	5.135	1257	1258	1260	rVB	188	64	0.00%	0.001%
30	5.148	1260	1262	1267	rBV2	290	226	0.01%	0.002%
31	5.174	1267	1270	1271	rBV	196	95	0.01%	0.001%
32	5.203	1276	1279	1282	rBV2	165	119	0.01%	0.001%
33	5.216	1282	1283	1285	rBV	304	106	0.01%	0.001%
34	5.315	1290	1314	1346	rBV2	538632	1599977	100.00%	13.288%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033882.D
 Acq On : 21 Aug 2019 19:21
 Operator : JC/SP
 Sample : K4420-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2C07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

35	5.766	1452	1454	1457	rBV2	373	184	0.01%	0.002%
36	5.865	1467	1485	1513	rBV	469169	942562	58.91%	7.828%
37	6.161	1565	1577	1594	rVB8	13311	31716	1.98%	0.263%
38	6.245	1601	1603	1605	rBV	281	141	0.01%	0.001%
39	6.309	1608	1623	1648	rBV	364484	738458	46.15%	6.133%
40	6.621	1717	1720	1723	rBV2	280	255	0.02%	0.002%
41	6.653	1728	1730	1734	rVB	333	141	0.01%	0.001%
42	6.672	1734	1736	1740	rVB	192	77	0.00%	0.001%
43	6.698	1740	1744	1747	rVB3	392	266	0.02%	0.002%
44	6.717	1747	1750	1752	rBV2	141	92	0.01%	0.001%
45	6.733	1752	1755	1764	rVB3	525	496	0.03%	0.004%
46	6.814	1778	1780	1784	rVB	337	197	0.01%	0.002%
47	6.836	1784	1787	1790	rBV2	428	397	0.02%	0.003%
48	6.965	1822	1827	1829	rBV	220	223	0.01%	0.002%
49	7.003	1836	1839	1841	rBV	241	166	0.01%	0.001%
50	7.074	1857	1861	1862	rBV	311	216	0.01%	0.002%
51	7.119	1871	1875	1879	rBV3	165	126	0.01%	0.001%
52	7.138	1879	1881	1882	rBV	315	83	0.01%	0.001%
53	7.164	1885	1889	1890	rBV2	300	185	0.01%	0.002%
54	7.209	1890	1903	1924	rBV	175374	320237	20.02%	2.660%
55	7.547	1995	2008	2040	rBV	700227	1227421	76.71%	10.194%
56	7.833	2085	2097	2127	rBV	123128	227777	14.24%	1.892%
57	8.026	2155	2157	2159	rVB2	528	199	0.01%	0.002%
58	8.126	2185	2188	2191	rBV	235	150	0.01%	0.001%
59	8.142	2191	2193	2195	rBV	291	137	0.01%	0.001%
60	8.203	2211	2212	2213	rBV	269	56	0.00%	0.000%
61	8.293	2229	2240	2274	rBV	360140	713552	44.60%	5.926%
62	8.569	2322	2326	2329	rBV3	534	469	0.03%	0.004%
63	8.685	2356	2362	2367	rBV5	659	836	0.05%	0.007%
64	8.769	2383	2388	2391	rVB	708	466	0.03%	0.004%
65	8.794	2393	2396	2397	rBV2	224	123	0.01%	0.001%
66	8.810	2397	2401	2402	rBV	519	354	0.02%	0.003%
67	8.920	2432	2435	2437	rBV	252	130	0.01%	0.001%
68	9.026	2465	2468	2469	rBV2	213	138	0.01%	0.001%
69	9.071	2469	2482	2512	rBV	715630	1210538	75.66%	10.054%
70	9.283	2546	2548	2551	rVB	668	334	0.02%	0.003%
71	9.299	2551	2553	2555	rBV	620	393	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033882.D
 Acq On : 21 Aug 2019 19:21
 Operator : JC/SP
 Sample : K4420-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2C07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

72	9.611	2647	2650	2654	rBV2	406	311	0.02%	0.003%
73	9.849	2720	2724	2728	rBV2	355	366	0.02%	0.003%
74	9.910	2740	2743	2746	rVB2	378	200	0.01%	0.002%
75	9.926	2746	2748	2752	rBV2	437	303	0.02%	0.003%
76	9.942	2752	2753	2754	rBV2	234	79	0.00%	0.001%
77	10.222	2838	2840	2843	rVB2	470	252	0.02%	0.002%
78	10.415	2887	2900	2924	rBV	506470	822304	51.39%	6.829%
79	10.672	2978	2980	2983	rBV3	332	135	0.01%	0.001%
80	10.939	3059	3063	3068	rBV2	427	505	0.03%	0.004%
81	10.984	3075	3077	3083	rBV	324	352	0.02%	0.003%
82	11.032	3090	3092	3093	rBV	369	185	0.01%	0.002%
83	11.151	3127	3129	3130	rBV	261	99	0.01%	0.001%
84	11.402	3205	3207	3211	rBV2	352	201	0.01%	0.002%
85	11.466	3215	3227	3249	rBV	617016	992122	62.01%	8.240%
86	11.842	3332	3344	3370	rBV	658278	1079263	67.45%	8.964%
87	12.267	3473	3476	3480	rBV2	911	710	0.04%	0.006%


Sum of corrected areas: 12040595

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082119\
Data File : VU033882.D
Acq On : 21 Aug 2019 19:21
Operator : JC/SP
Sample : K4420-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
F2C07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

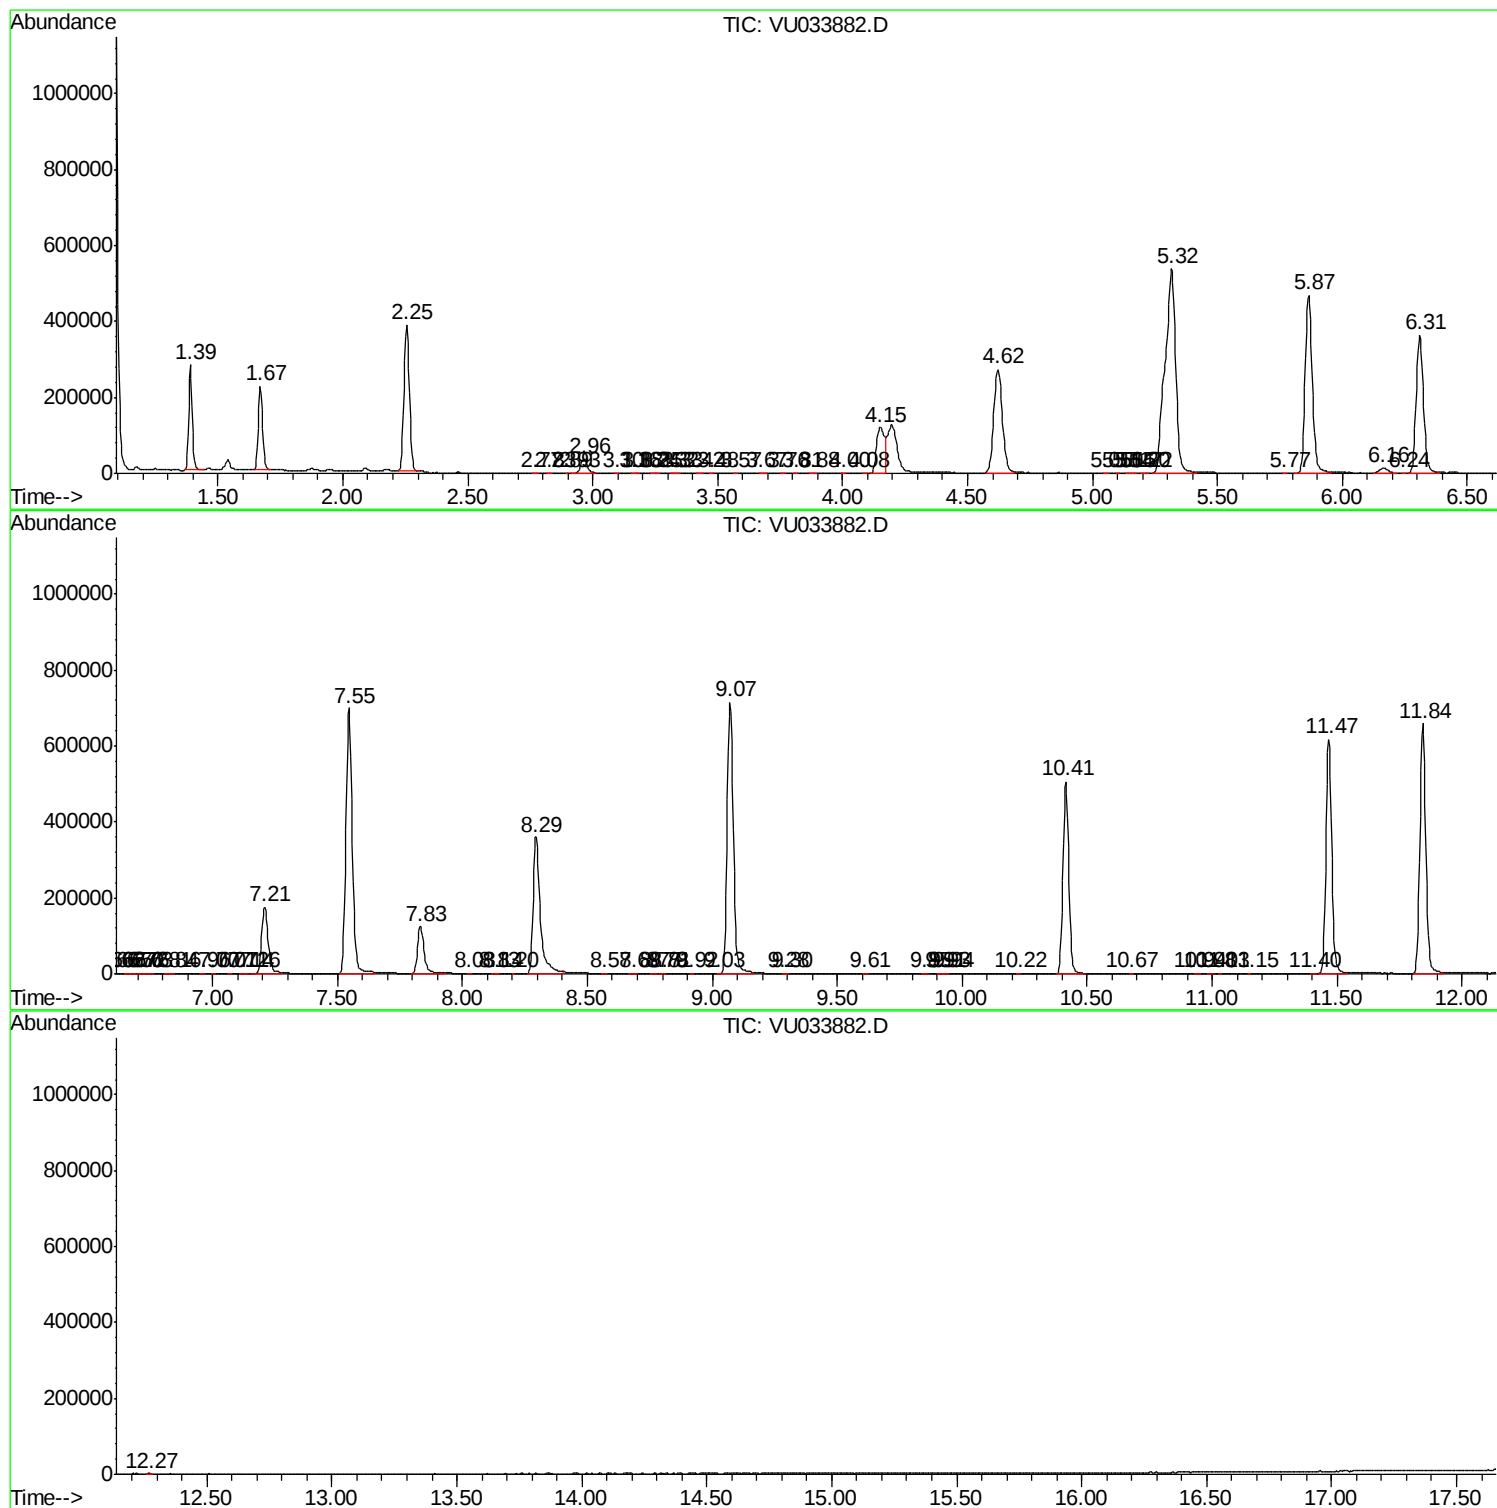

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082119\
Data File : VU033882.D
Acq On : 21 Aug 2019 19:21
Operator : JC/SP
Sample : K4420-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2C07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082119\
Data File : VU033882.D
Acq On : 21 Aug 2019 19:21
Operator : JC/SP
Sample : K4420-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2C07

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc