

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033886.D
 Acq On : 21 Aug 2019 20:56
 Operator : JC/SP
 Sample : K4420-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	86	93	106	rVB	236951	253217	16.48%	2.128%
2	1.669	173	180	197	rVB	206069	254583	16.57%	2.140%
3	2.254	353	362	377	rVB	344602	519601	33.82%	4.367%
4	2.762	518	520	522	rBV2	264	113	0.01%	0.001%
5	2.781	522	526	530	rBV5	342	365	0.02%	0.003%
6	2.804	530	533	538	rBV3	909	1004	0.07%	0.008%
7	2.916	566	568	573	rVB2	368	244	0.02%	0.002%
8	2.939	573	575	576	rVV	313	155	0.01%	0.001%
9	2.965	580	583	589	rVB3	1115	1033	0.07%	0.009%
10	3.000	590	594	597	rBV2	185	179	0.01%	0.002%
11	3.058	609	612	619	rVB	481	405	0.03%	0.003%
12	3.090	619	622	626	rVB2	354	221	0.01%	0.002%
13	3.112	626	629	632	rBV2	308	265	0.02%	0.002%
14	3.170	642	647	649	rBV	376	339	0.02%	0.003%
15	3.219	659	662	667	rVB2	334	261	0.02%	0.002%
16	3.260	672	675	681	rVV2	349	403	0.03%	0.003%
17	3.283	681	682	686	rVB2	235	127	0.01%	0.001%
18	3.305	686	689	690	rBV	276	145	0.01%	0.001%
19	3.315	690	692	695	rVB	96	68	0.00%	0.001%
20	3.347	700	702	704	rVV2	264	113	0.01%	0.001%
21	3.386	712	714	718	rBV2	182	140	0.01%	0.001%
22	3.437	725	730	733	rBV2	328	317	0.02%	0.003%
23	3.524	755	757	758	rBV	75	32	0.00%	0.000%
24	3.534	758	760	762	rBV	189	107	0.01%	0.001%
25	3.563	766	769	771	rBV	146	94	0.01%	0.001%
26	3.595	776	779	782	rBV2	166	114	0.01%	0.001%
27	3.611	782	784	788	rVB2	350	197	0.01%	0.002%
28	3.643	788	794	797	rBV2	346	380	0.02%	0.003%
29	3.665	797	801	803	rBV2	325	243	0.02%	0.002%
30	3.739	821	824	828	rBV2	232	264	0.02%	0.002%
31	3.791	837	840	843	rVB2	330	199	0.01%	0.002%
32	3.813	843	847	855	rVB2	313	322	0.02%	0.003%
33	3.849	855	858	860	rBV	157	117	0.01%	0.001%
34	3.913	876	878	880	rBV	161	89	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033886.D
 Acq On : 21 Aug 2019 20:56
 Operator : JC/SP
 Sample : K4420-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

35	3.936	882	885	888	rVB3	301	196	0.01%	0.002%
36	3.958	891	892	894	rBV	200	52	0.00%	0.000%
37	4.013	907	909	912	rBB	220	97	0.01%	0.001%
38	4.048	912	920	922	rBV3	499	515	0.03%	0.004%
39	4.096	933	935	938	rVB2	191	103	0.01%	0.001%
40	4.148	938	951	989	rBV	136029	383316	24.95%	3.221%
41	4.620	1081	1098	1125	rBV	269041	645151	42.00%	5.422%
42	4.845	1166	1168	1173	rBV4	665	610	0.04%	0.005%
43	4.900	1182	1185	1189	rVB2	952	750	0.05%	0.006%
44	4.926	1189	1193	1194	rBV	452	303	0.02%	0.003%
45	5.013	1218	1220	1223	rBV2	181	59	0.00%	0.000%
46	5.128	1254	1256	1259	rBV2	273	185	0.01%	0.002%
47	5.315	1291	1314	1344	rBV2	514957	1536220	100.00%	12.910%
48	5.630	1407	1412	1414	rBV	550	438	0.03%	0.004%
49	5.662	1419	1422	1423	rBV3	472	263	0.02%	0.002%
50	5.730	1440	1443	1450	rBV3	332	331	0.02%	0.003%
51	5.810	1466	1468	1470	rBV2	159	72	0.00%	0.001%
52	5.865	1470	1485	1510	rBV	462265	920655	59.93%	7.737%
53	6.157	1566	1576	1588	rBV7	7173	14942	0.97%	0.126%
54	6.308	1608	1623	1649	rBV	352146	711087	46.29%	5.976%
55	6.585	1706	1709	1711	rBV3	419	300	0.02%	0.003%
56	6.620	1719	1720	1726	rBV2	201	127	0.01%	0.001%
57	6.659	1731	1732	1734	rVV	373	90	0.01%	0.001%
58	6.678	1735	1738	1742	rVB	318	230	0.01%	0.002%
59	6.804	1767	1777	1786	rBV5	3986	7197	0.47%	0.060%
60	6.849	1789	1791	1792	rBV	489	238	0.02%	0.002%
61	6.900	1804	1807	1808	rBV	203	85	0.01%	0.001%
62	6.916	1808	1812	1813	rBV	200	146	0.01%	0.001%
63	6.958	1823	1825	1827	rBV	363	196	0.01%	0.002%
64	7.048	1851	1853	1857	rVB	588	346	0.02%	0.003%
65	7.070	1857	1860	1863	rBV2	269	185	0.01%	0.002%
66	7.087	1863	1865	1866	rVV2	188	57	0.00%	0.000%
67	7.122	1874	1876	1879	rBV	168	95	0.01%	0.001%
68	7.209	1891	1903	1925	rBV	171942	320222	20.84%	2.691%
69	7.476	1985	1986	1988	rVB	335	88	0.01%	0.001%
70	7.546	1995	2008	2028	rBV	658246	1147834	74.72%	9.646%
71	7.832	2086	2097	2116	rBV	124245	216810	14.11%	1.822%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082119\
 Data File : VU033886.D
 Acq On : 21 Aug 2019 20:56
 Operator : JC/SP
 Sample : K4420-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis

72	8.054	2164	2166	2167	rBV	260	68	0.00%	0.001%
73	8.067	2168	2170	2172	rVV2	218	95	0.01%	0.001%
74	8.144	2192	2194	2199	rBV2	433	279	0.02%	0.002%
75	8.173	2199	2203	2206	rBV2	319	245	0.02%	0.002%
76	8.244	2222	2225	2228	rBV	169	136	0.01%	0.001%
77	8.296	2228	2241	2276	rBV	428213	831261	54.11%	6.986%
78	8.778	2389	2391	2393	rBV	143	96	0.01%	0.001%
79	8.800	2396	2398	2399	rVV	168	51	0.00%	0.000%
80	8.861	2413	2417	2419	rBV2	273	198	0.01%	0.002%
81	8.897	2426	2428	2432	rVB	537	270	0.02%	0.002%
82	8.926	2432	2437	2440	rBV2	379	271	0.02%	0.002%
83	9.070	2467	2482	2508	rBV	710160	1200094	78.12%	10.086%
84	9.328	2560	2562	2564	rBV2	413	166	0.01%	0.001%
85	9.360	2568	2572	2574	rBV3	1419	1090	0.07%	0.009%
86	9.476	2606	2608	2613	rBV3	299	209	0.01%	0.002%
87	9.530	2621	2625	2628	rBV3	437	296	0.02%	0.002%
88	9.604	2646	2648	2650	rBV	307	143	0.01%	0.001%
89	9.649	2659	2662	2664	rBV2	340	144	0.01%	0.001%
90	9.813	2711	2713	2715	rBV3	240	128	0.01%	0.001%
91	10.080	2793	2796	2799	rBV2	255	131	0.01%	0.001%
92	10.096	2799	2801	2802	rBV	182	45	0.00%	0.000%
93	10.138	2810	2814	2816	rBV2	326	236	0.02%	0.002%
94	10.353	2877	2881	2882	rBV2	376	216	0.01%	0.002%
95	10.414	2888	2900	2929	rVB	523731	845894	55.06%	7.109%
96	10.726	2995	2997	2999	rBV2	188	62	0.00%	0.001%
97	10.752	2999	3005	3010	rBV3	845	923	0.06%	0.008%
98	11.421	3211	3213	3215	rBV2	502	202	0.01%	0.002%
99	11.466	3215	3227	3253	rBV	610397	1009569	65.72%	8.484%
100	11.842	3332	3344	3373	rBV	638110	1061573	69.10%	8.921%


Sum of corrected areas: 11899138

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082119\
Data File : VU033886.D
Acq On : 21 Aug 2019 20:56
Operator : JC/SP
Sample : K4420-18
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

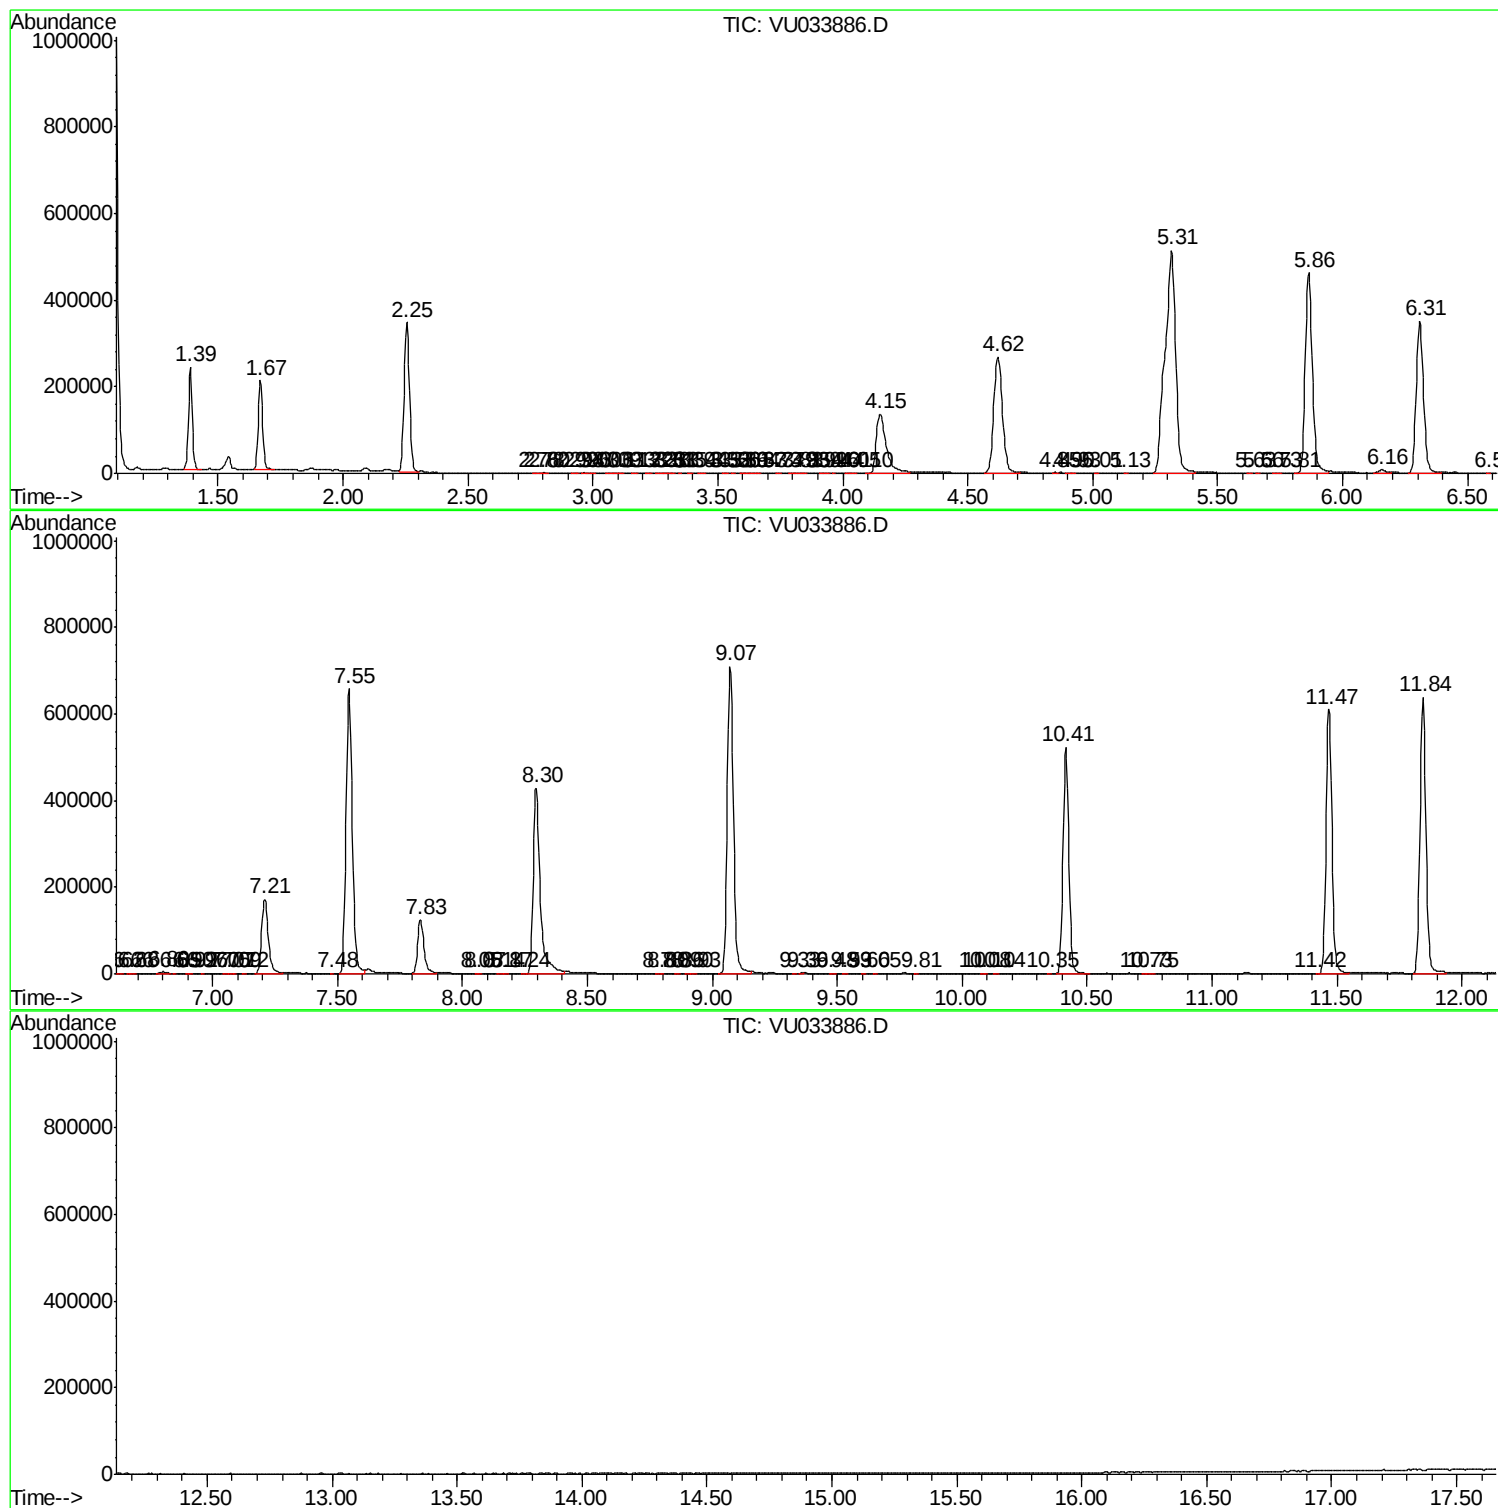

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082119\
Data File : VU033886.D
Acq On : 21 Aug 2019 20:56
Operator : JC/SP
Sample : K4420-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082119\
Data File : VU033886.D
Acq On : 21 Aug 2019 20:56
Operator : JC/SP
Sample : K4420-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc