


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082119\
 Data File : VU033861.D
 Acq On : 21 Aug 2019 10:16
 Operator : JC/SP
 Sample : BFB59
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB59

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM081619WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 22 07:18:35 2019

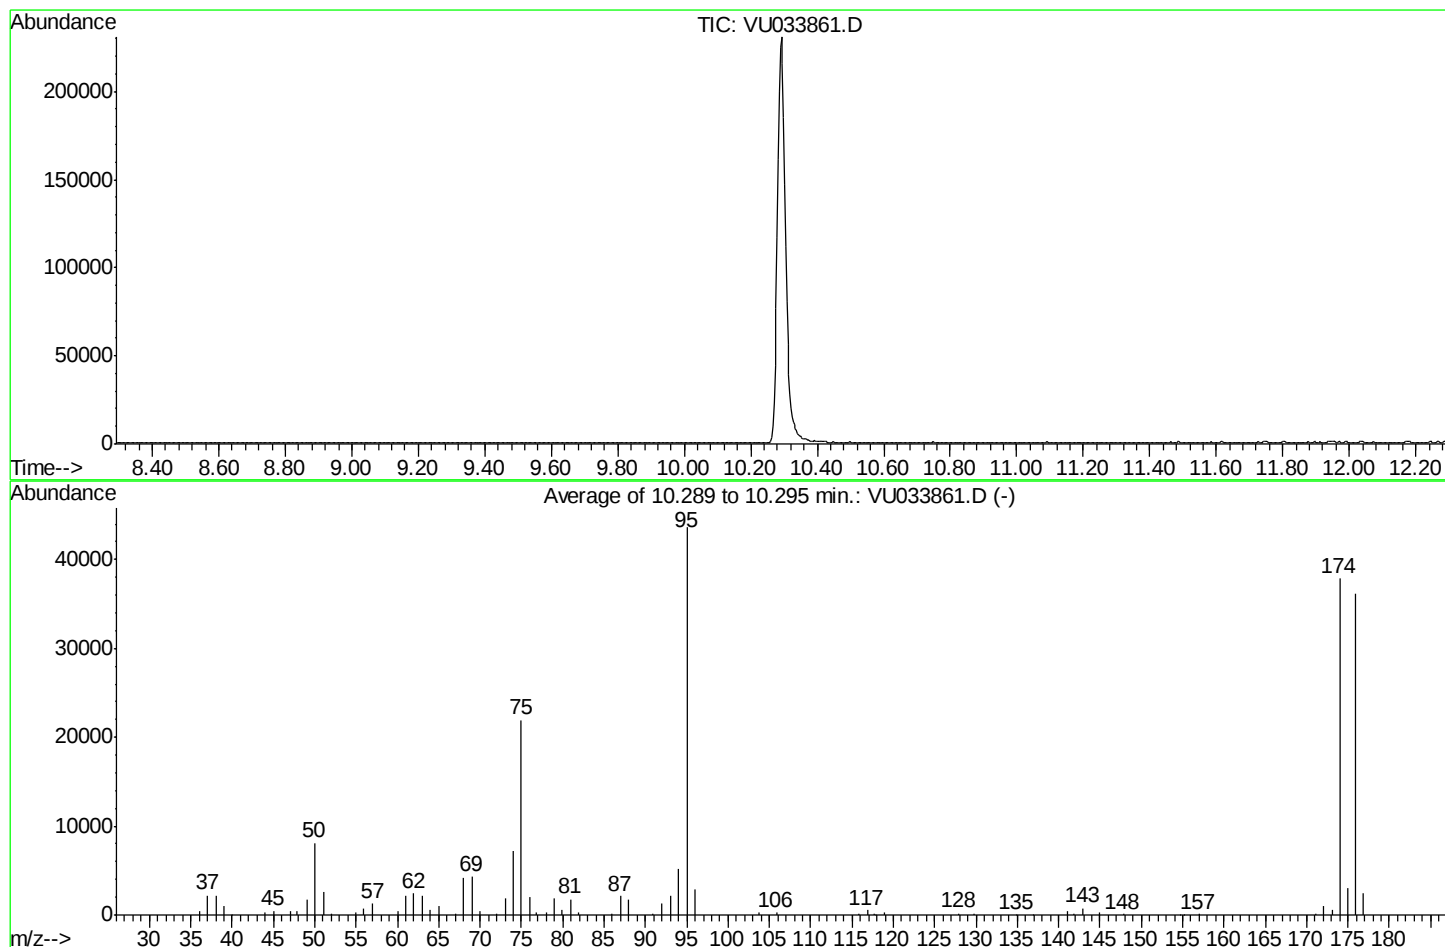

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	8101	PASS
75	95	30	80	50.2	21920	PASS
95	95	100	100	100.0	43629	PASS
96	95	5	9	6.8	2952	PASS
173	174	0.00	2	1.4	526	PASS
174	95	50	120	86.7	37834	PASS
175	174	5	9	8.1	3051	PASS
176	174	95	101	95.7	36194	PASS
177	176	5	9	6.9	2515	PASS

m/z	Abundance
36.00	445.0
37.00	2296.0
38.00	2336.0
39.00	1021.0
40.00	316.0
44.00	726.0
45.00	482.0
47.00	513.0
47.90	406.0
49.00	1826.0
50.00	8503.0
51.10	2651.0
51.90	161.0
55.00	254.0
56.00	788.0
57.00	1310.0
60.00	426.0
61.00	2228.0
62.00	2485.0
63.10	2231.0
63.90	537.0
65.00	915.0
67.00	159.0
68.00	4402.0
69.00	4464.0
70.10	525.0
72.00	180.0
73.00	1877.0
74.00	7401.0
75.00	21936.0
76.00	2100.0
76.90	329.0
78.00	260.0
78.90	1803.0
79.90	600.0
80.90	1736.0
82.00	277.0
85.80	144.0
87.00	2128.0
88.00	1681.0
90.90	238.0
92.00	1279.0
93.00	2227.0
94.00	5104.0
95.00	44808.0
96.00	2948.0
103.80	265.0
105.80	212.0
115.90	121.0
116.90	510.0
117.70	218.0
118.90	265.0
127.90	156.0
129.70	117.0
134.90	113.0
136.90	103.0
141.00	473.0
141.90	104.0
143.00	747.0
144.90	261.0
147.80	130.0
154.70	137.0
156.90	129.0
172.00	975.0
174.00	37352.0
174.90	3187.0
175.90	35416.0
176.90	2534.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	491.0
37.00	2238.0
38.10	2205.0
39.00	982.0
39.90	330.0
44.00	792.0
45.00	512.0
47.00	515.0
47.90	415.0
49.00	1855.0
50.00	8382.0
51.10	2668.0
52.00	154.0
55.00	248.0
56.00	826.0
57.00	1253.0
60.00	469.0
61.00	2234.0
62.00	2467.0
63.10	2260.0
63.90	535.0
65.00	1030.0
67.10	198.0
68.00	4396.0
69.00	4447.0
70.00	499.0
71.90	170.0
73.00	2024.0
74.00	7381.0
75.00	22632.0
76.00	2051.0
76.90	278.0
78.00	292.0
78.90	1948.0
79.90	600.0
80.90	1801.0
82.00	311.0
85.90	125.0
87.00	2169.0
88.00	1739.0
90.90	234.0
92.00	1332.0
93.00	2168.0
94.00	5278.0
95.00	45024.0
96.10	3051.0
103.80	227.0
105.80	222.0
115.90	134.0
116.90	598.0
117.70	220.0
119.00	321.0
127.90	169.0
129.80	108.0
134.90	114.0
141.00	459.0
141.80	121.0
143.00	775.0
145.00	259.0
147.80	110.0
157.00	137.0
171.10	175.0
172.00	1079.0
173.10	755.0
174.00	38848.0
174.90	3188.0
175.90	37280.0
176.90	2652.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	510.0
37.00	2049.0
38.10	1787.0
39.00	847.0
39.90	364.0
44.00	811.0
45.00	420.0
47.00	474.0
47.90	350.0
49.00	1722.0
50.00	7419.0
51.10	2386.0
52.00	110.0
54.90	200.0
55.90	726.0
57.00	1133.0
60.00	425.0
61.00	1990.0
62.00	2229.0
63.00	2129.0
64.00	468.0
65.00	972.0
67.10	176.0
68.00	3917.0
69.00	4047.0
69.90	446.0
71.90	195.0
73.00	1945.0
74.10	6994.0
75.00	21192.0
76.00	1818.0
76.80	277.0
78.00	251.0
78.90	1889.0
79.90	465.0
80.90	1746.0
81.90	327.0
85.90	131.0
87.00	2004.0
88.00	1679.0
90.90	158.0
92.00	1262.0
93.00	1916.0
94.00	5007.0
95.00	41056.0
96.00	2857.0
103.70	183.0
105.90	255.0
115.80	122.0
116.90	548.0
117.90	196.0
119.00	360.0
127.90	191.0
129.70	101.0
141.00	409.0
141.80	111.0
142.90	725.0
145.00	295.0
147.80	102.0
155.10	100.0
157.00	116.0
171.00	131.0
172.00	1096.0
173.10	824.0
174.00	37304.0
175.00	2779.0
176.00	35888.0
176.90	2359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

Scan 2850 (10.254 min): VU033861.D
BFB59

m/z	Abundance
39.90	295.0
44.00	433.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59