


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082120\
Data File : VU039936.D
Acq On : 21 Aug 2020 18:26
Operator : SY/MD
Sample : L3776-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 22 02:41:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 22 00:45:05 2020
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampled :
F4Y12

Manual Integrations
APPROVED

sam
8/24/2020 5:55:37 PM

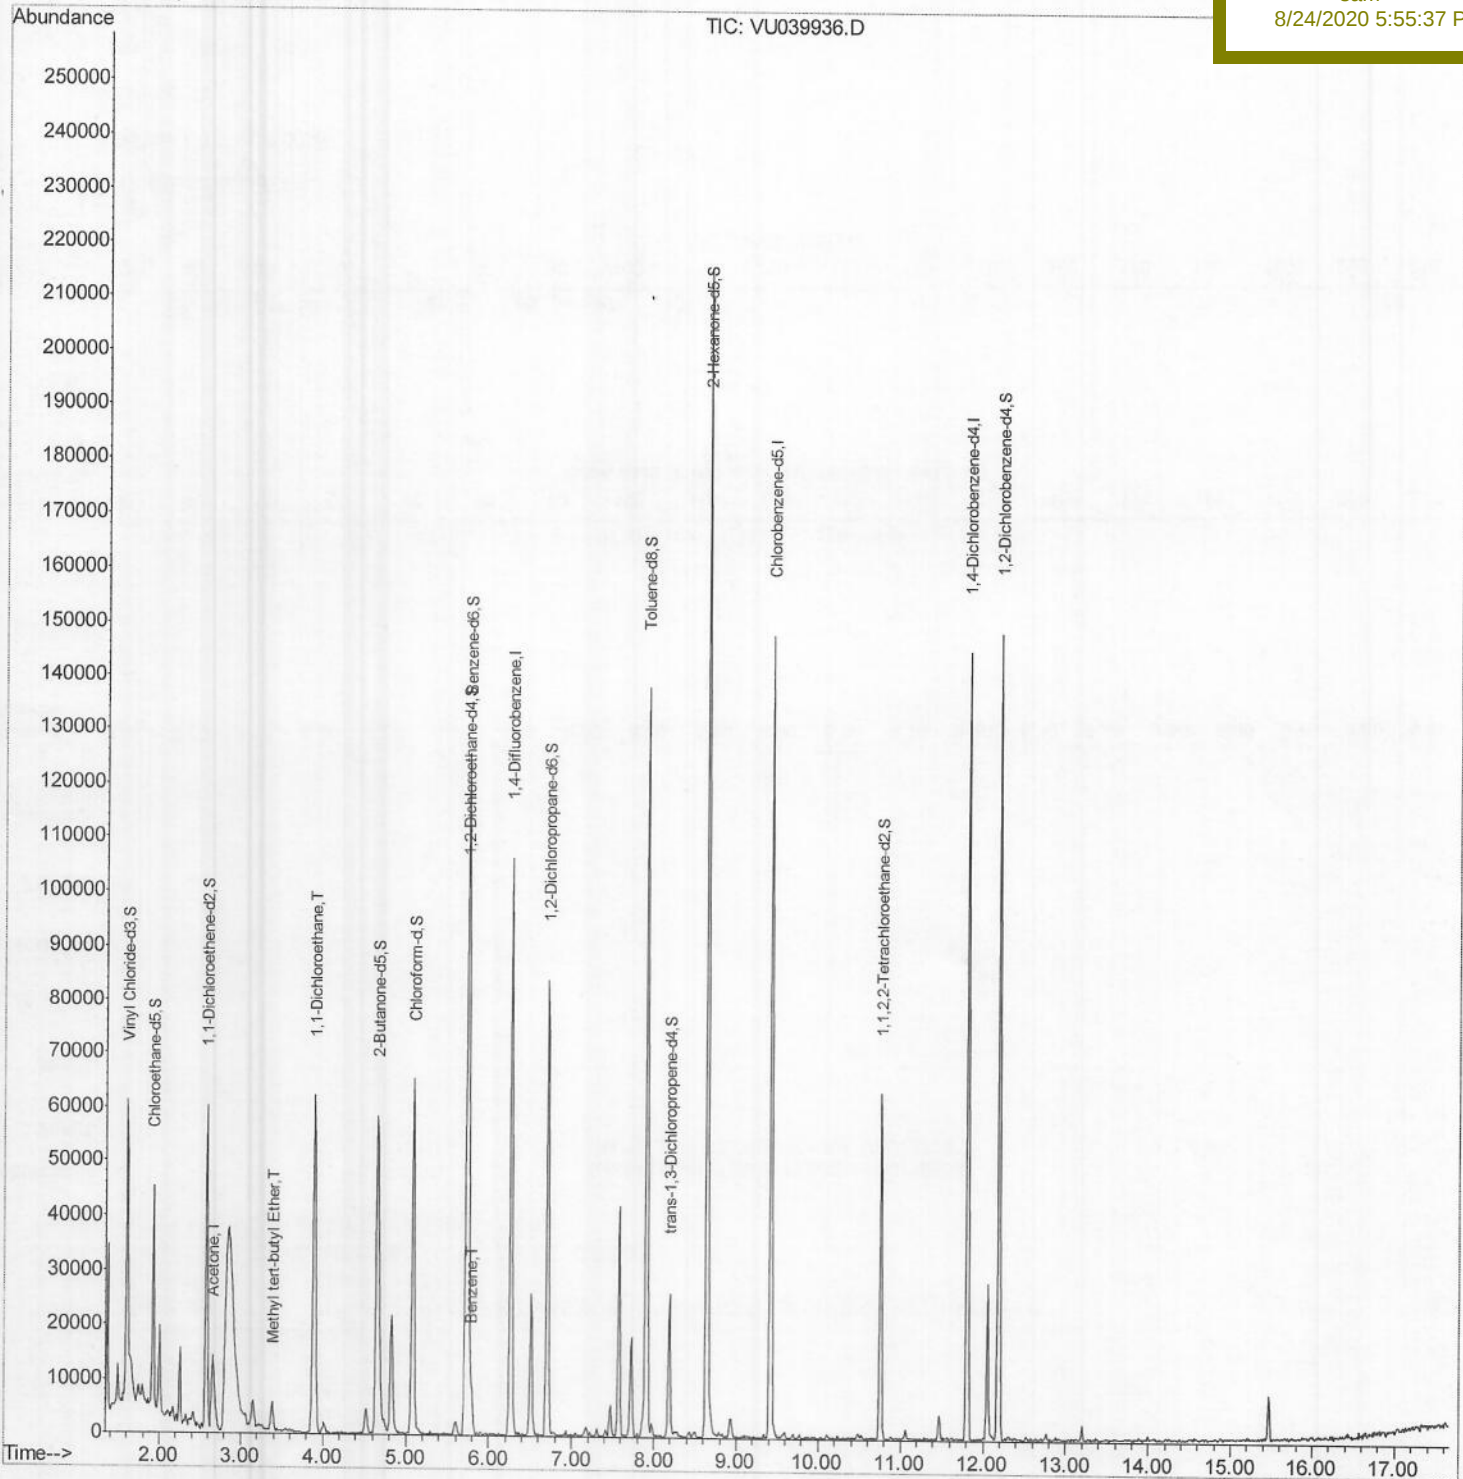

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082120\

Data File : VU039936.D

Acq On : 21 Aug 2020 18:26

Operator : SY/MD

Sample : L3776-13

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 22 00:49:38 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Aug 22 00:45:05 2020

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :




F4Y12

Manual Integrations

APPROVED

sam

8/24/2020 5:55:37 PM

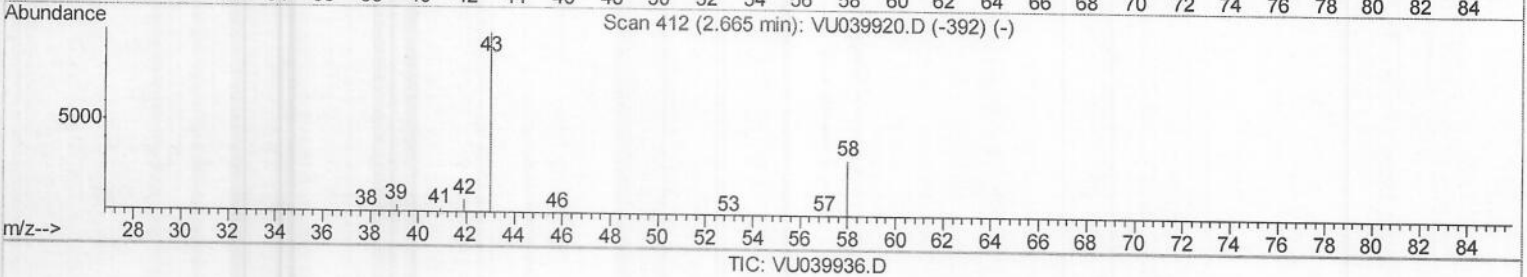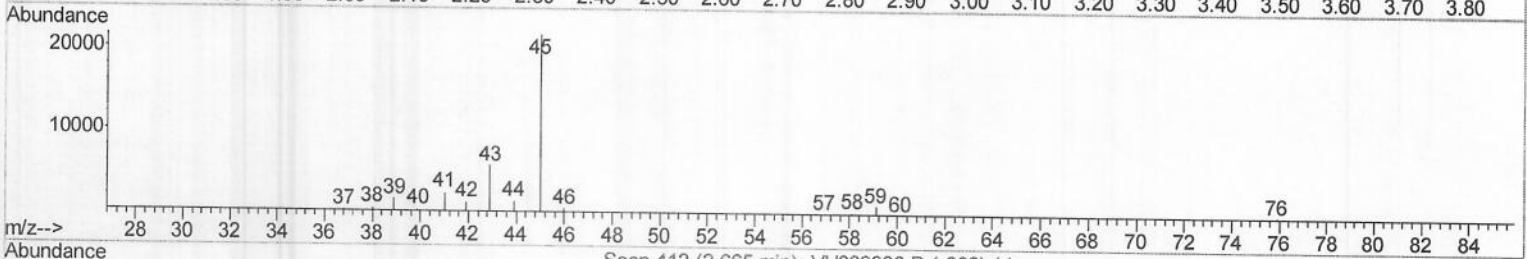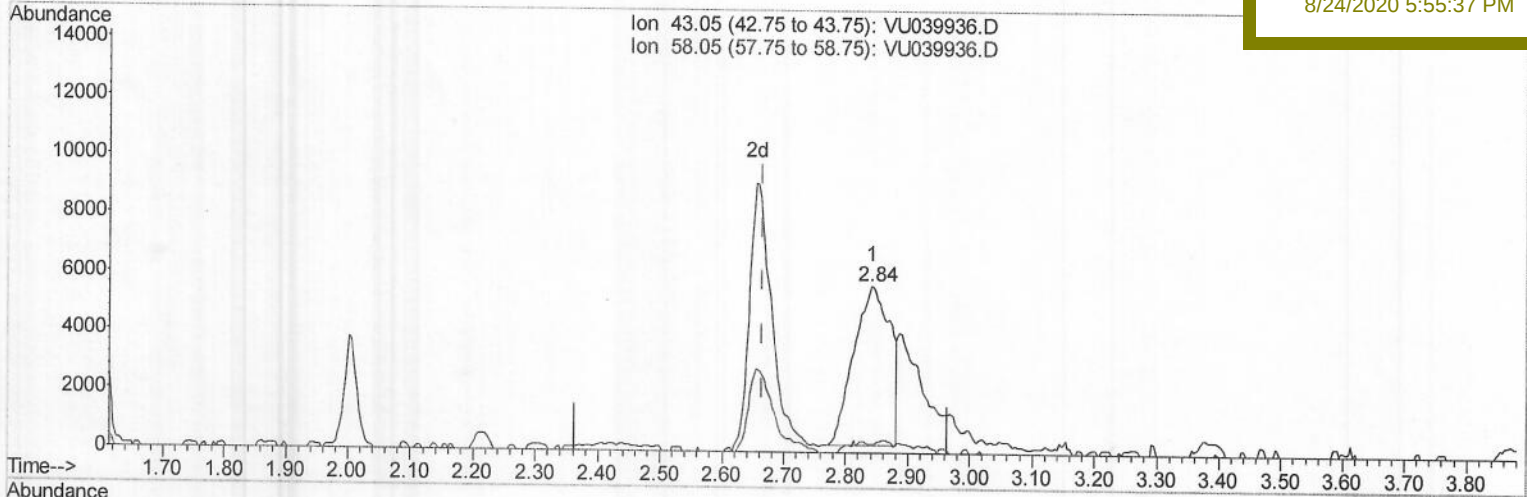

(13) Acetone (T)

2.842min (+0.177) 14.31ug/L

response 21659

Ion	Exp%	Act%
43.05	100	100
58.05	9.50	1.94
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082120\

Data File : VU039936.D

Acq On : 21 Aug 2020 18:26

Operator : SY/MD

Sample : L3776-13

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 22 00:49:38 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Aug 22 00:45:05 2020

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleID :




F4Y12

Manual Integrations

APPROVED

sam

8/24/2020 5:55:37 PM

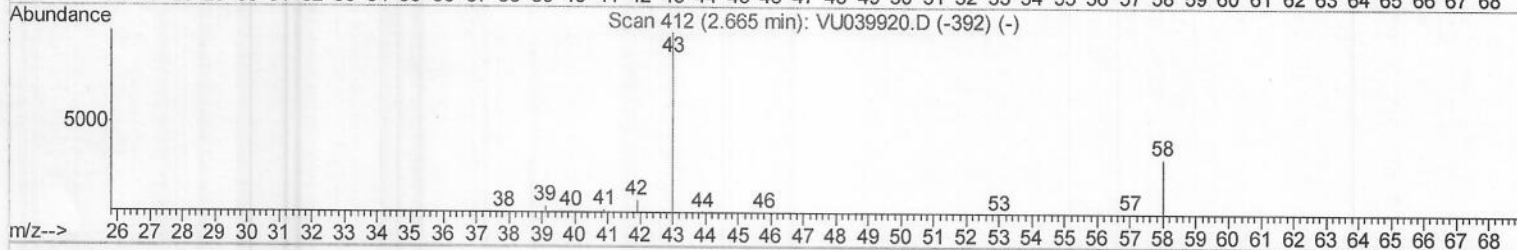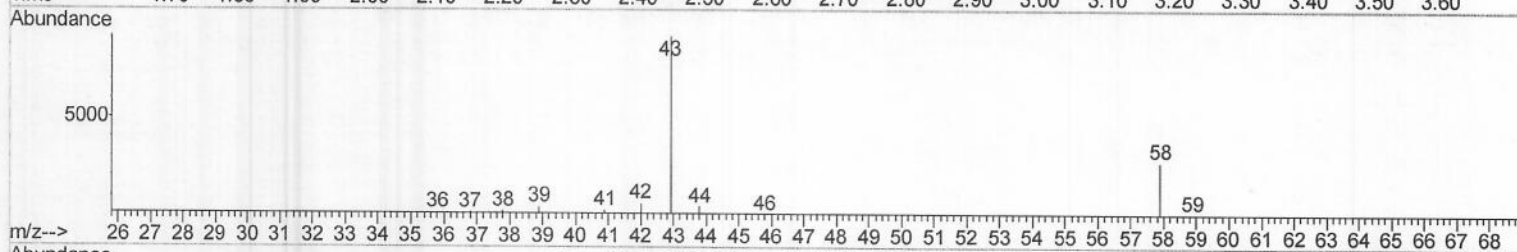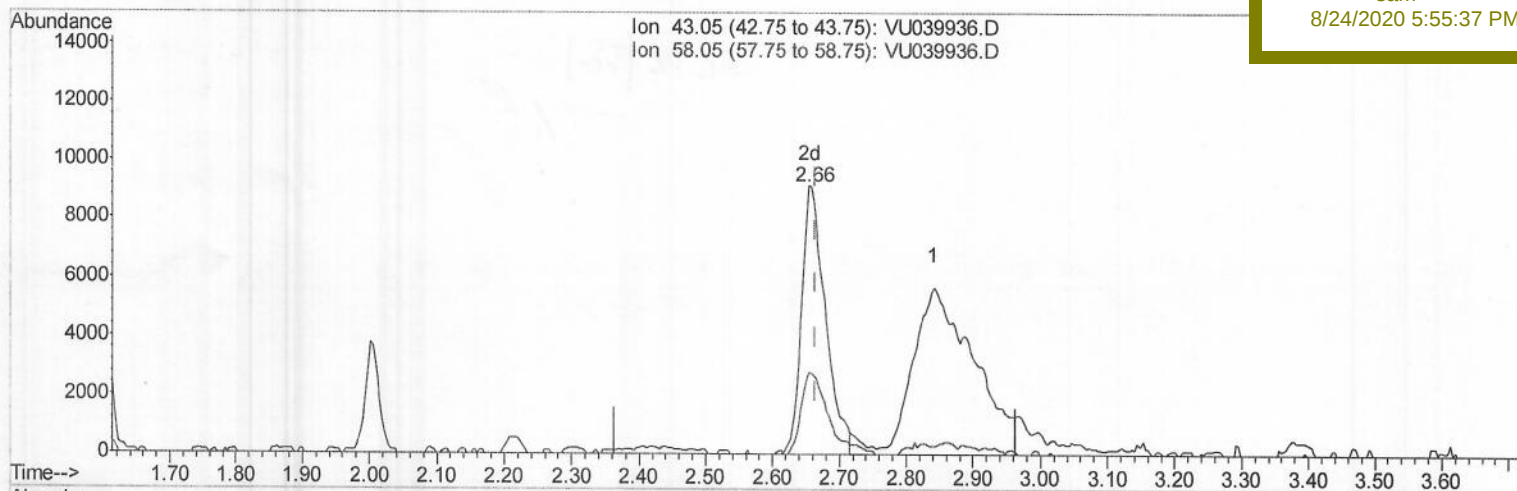

TIC: VU039936.D

(13) Acetone (T)

2.655min (-0.010) 14.93ug/L m > 57 08/24/20

response 22596

Ion	Exp%	Act%
43.05	100	100
58.05	9.50	1.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082120\
 Data File : VU039936.D
 Acq On : 21 Aug 2020 18:26
 Operator : SY/MD
 Sample : L3776-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4Y12

Quant Time: Aug 22 02:41:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 22 00:45:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sam
 8/24/2020 5:55:37 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	79352	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	70892	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	34698	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	27013	3.90	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.00%	
7) Chloroethane-d5	1.92	69	25429	4.43	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.60%	
11) 1,1-Dichloroethene-d2	2.58	63	36404	2.72	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	54.40%#	
20) 2-Butanone-d5	4.65	46	101813	45.96	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	91.92%	
24) Chloroform-d	5.08	84	56405	4.51	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.20%	
26) 1,2-Dichloroethane-d4	5.72	65	32016	4.32	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.40%	
32) Benzene-d6	5.74	84	107651	5.10	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.00%	
36) 1,2-Dichloropropane-d6	6.70	67	36233	5.20	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.00%	
41) Toluene-d8	7.91	98	83861	4.54	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.80%	
43) trans-1,3-Dichloropropene-	8.19	79	12241	4.19	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.80%	
46) 2-Hexanone-d5	8.64	63	69190	46.67	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.34%	
57) 1,1,2,2-Tetrachloroethane-	10.75	84	29048	4.70	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.00%	
64) 1,2-Dichlorobenzene-d4	12.19	152	35034	5.12	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.40%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.66	43	22596m	14.929	ug/L	
17) Methyl tert-butyl Ether	3.38	73	5158	0.295	ug/L	# 82
19) 1,1-Dichloroethane	3.89	63	66119	4.948	ug/L	99
33) Benzene	5.79	78	7723	0.300	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

15X 08/24/20