


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082120\
 Data File : VU039919.D
 Acq On : 21 Aug 2020 09:27
 Operator : SY/MD
 Sample : BFB18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 24 15:44:09 2020

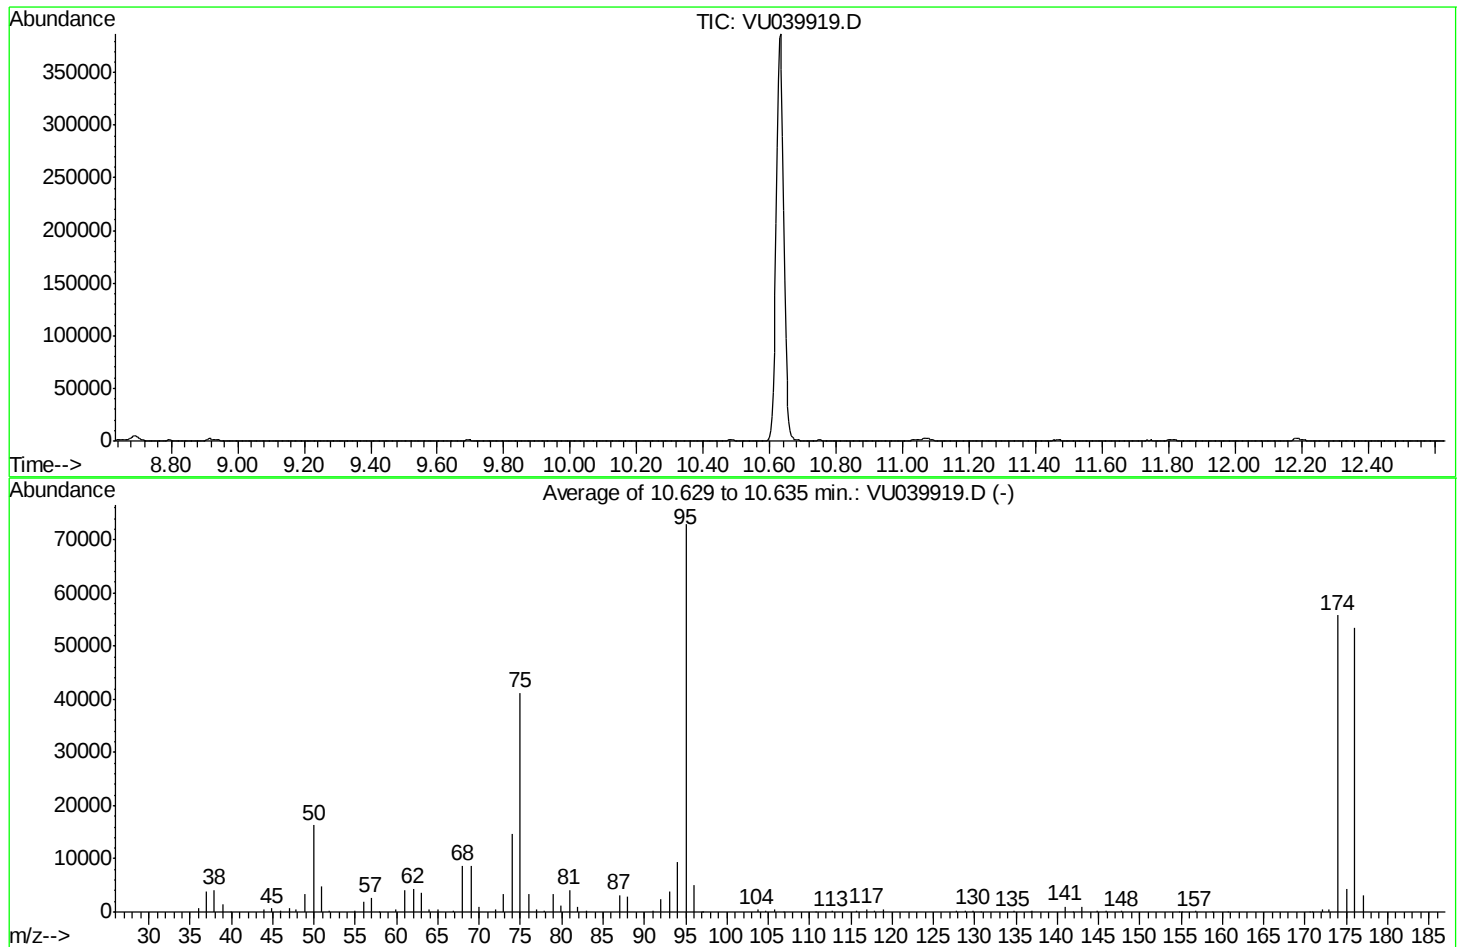

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	16288	PASS
75	95	30	80	56.5	41189	PASS
95	95	100	100	100.0	72909	PASS
96	95	5	9	6.8	4966	PASS
173	174	0.00	2	1.0	569	PASS
174	95	50	120	76.6	55834	PASS
175	174	5	9	7.8	4337	PASS
176	174	95	101	95.7	53461	PASS
177	176	5	9	5.9	3180	PASS

m/z	Abundance
35.90	603.0
37.00	4152.0
37.90	4381.0
39.00	1751.0
39.90	125.0
44.00	884.0
44.90	746.0
45.80	124.0
47.00	856.0
47.80	464.0
48.90	3819.0
50.00	17000.0
51.00	5198.0
51.90	268.0
55.00	374.0
56.00	1868.0
57.00	2986.0
57.90	136.0
60.00	710.0
61.00	3995.0
62.00	4581.0
63.00	3999.0
63.90	486.0
65.00	406.0
66.90	281.0
68.00	8617.0
69.00	8997.0
70.00	927.0
72.00	477.0
72.90	3472.0
74.00	15114.0
75.00	43016.0
76.00	3422.0
77.00	496.0
77.80	392.0
78.90	3534.0
79.90	1204.0
80.90	4043.0
81.90	1062.0
83.00	171.0
87.00	3080.0
87.90	3076.0
91.10	279.0
92.00	2418.0
93.00	4086.0
94.00	9413.0
95.00	75344.0
96.00	5264.0
96.90	169.0
103.70	482.0
104.80	156.0
105.80	402.0
106.80	110.0
110.80	104.0
112.70	161.0
115.70	265.0
117.00	649.0
117.80	290.0
118.90	429.0
127.80	258.0
128.90	129.0
129.90	236.0
134.70	241.0
137.00	168.0
141.00	1064.0
141.90	106.0
142.90	939.0
144.70	202.0
145.90	134.0
147.90	202.0
154.80	117.0
156.70	201.0
160.70	114.0
170.60	157.0
172.10	515.0
173.00	545.0
174.00	55480.0
175.00	4497.0
176.00	53040.0
177.00	3204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	657.0
37.00	4100.0
38.00	4347.0
39.00	1570.0
40.00	119.0
44.00	775.0
44.90	684.0
45.90	141.0
46.90	770.0
47.80	522.0
48.90	3488.0
50.00	16840.0
51.00	5049.0
51.80	229.0
55.00	314.0
56.00	1909.0
56.90	2829.0
59.90	578.0
61.00	4110.0
62.00	4498.0
63.00	3887.0
63.90	443.0
65.00	435.0
66.90	272.0
68.00	9118.0
69.00	8958.0
70.00	927.0
72.00	566.0
73.00	3572.0
74.00	15129.0
75.00	42408.0
76.00	3481.0
77.00	457.0
77.80	319.0
78.90	3583.0
79.90	1144.0
80.90	4309.0
81.90	1097.0
83.00	196.0
87.00	3253.0
87.90	2916.0
91.10	283.0
92.00	2617.0
93.00	4079.0
94.00	9500.0
95.00	75608.0
96.00	5082.0
96.90	187.0
103.70	438.0
104.70	157.0
105.80	394.0
106.80	116.0
112.70	139.0
115.80	274.0
117.00	633.0
117.80	358.0
118.90	439.0
127.80	254.0
128.90	178.0
129.80	258.0
134.80	245.0
137.00	161.0
141.00	1069.0
142.00	121.0
142.90	924.0
144.80	200.0
145.90	149.0
147.80	155.0
154.80	140.0
156.80	204.0
158.70	101.0
170.60	149.0
172.00	523.0
172.80	583.0
174.00	57904.0
175.00	4483.0
176.00	55256.0
177.00	3291.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	647.0
37.00	3538.0
38.00	3808.0
39.00	1232.0
40.00	102.0
43.90	697.0
44.90	586.0
46.00	172.0
46.90	722.0
47.80	464.0
48.90	2808.0
50.00	15025.0
50.90	4437.0
51.90	199.0
55.00	223.0
55.90	1692.0
56.90	2506.0
59.80	444.0
61.00	3930.0
62.00	3946.0
63.00	3240.0
63.80	345.0
65.00	381.0
66.90	224.0
68.00	8513.0
69.00	7941.0
70.00	797.0
72.00	523.0
73.00	3335.0
74.00	13640.0
75.00	38144.0
76.00	3306.0
77.00	403.0
77.80	292.0
78.90	3169.0
79.80	977.0
80.90	3986.0
81.90	945.0
82.90	161.0
87.00	3100.0
87.90	2657.0
90.90	270.0
92.00	2539.0
93.00	3591.0
94.00	8982.0
95.00	67776.0
96.00	4554.0
97.10	203.0
103.70	342.0
104.70	125.0
105.80	359.0
112.80	119.0
115.80	291.0
116.90	553.0
117.90	395.0
118.90	403.0
127.80	223.0
128.80	238.0
129.80	284.0
130.80	100.0
134.80	219.0
136.70	118.0
137.00	119.0
141.00	1011.0
142.00	119.0
142.90	948.0
144.90	153.0
145.90	130.0
147.80	129.0
155.00	162.0
156.80	162.0
158.80	117.0
170.80	118.0
172.00	521.0
172.80	581.0
174.00	54120.0
175.00	4032.0
176.00	52088.0
177.00	3045.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
43.90	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18