

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
 Data File : VU026258.D
 Acq On : 22 Aug 2018 19:31
 Operator : MD/SY
 Sample : J4598-10 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBM9

Quant Time: Aug 23 07:28:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 23 07:27:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	296183	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	289475	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	136387	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	81080	44.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.76%
7) Chloroethane-d5	1.68	69	70984	48.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.38%
11) 1,1-Dichloroethene-d2	2.27	63	130464	36.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.48%
21) 2-Butanone-d5	4.18	46	157620	109.32	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.32%
24) Chloroform-d	4.65	84	197500	49.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.10%
26) 1,2-Dichloroethane-d4	5.31	65	132379	50.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.04%
32) Benzene-d6	5.35	84	379000	48.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.88%
36) 1,2-Dichloropropane-d6	6.34	67	124680	50.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.28%
41) Toluene-d8	7.57	98	346898	46.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.74%
43) trans-1,3-Dichloropropene-	7.85	79	59683	46.46	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.92%
47) 2-Hexanone-d5	8.31	63	109488	103.03	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.03%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	181820	49.41	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.82%
64) 1,2-Dichlorobenzene-d4	11.86	152	151028	52.19	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.38%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	11.48	75	14928	5.552 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
Data File : VU026258.D
Acq On : 22 Aug 2018 19:31
Operator : MD/SY
Sample : J4598-10 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBM9

Quant Time: Aug 23 07:28:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 23 07:27:18 2018
Response via : Initial Calibration

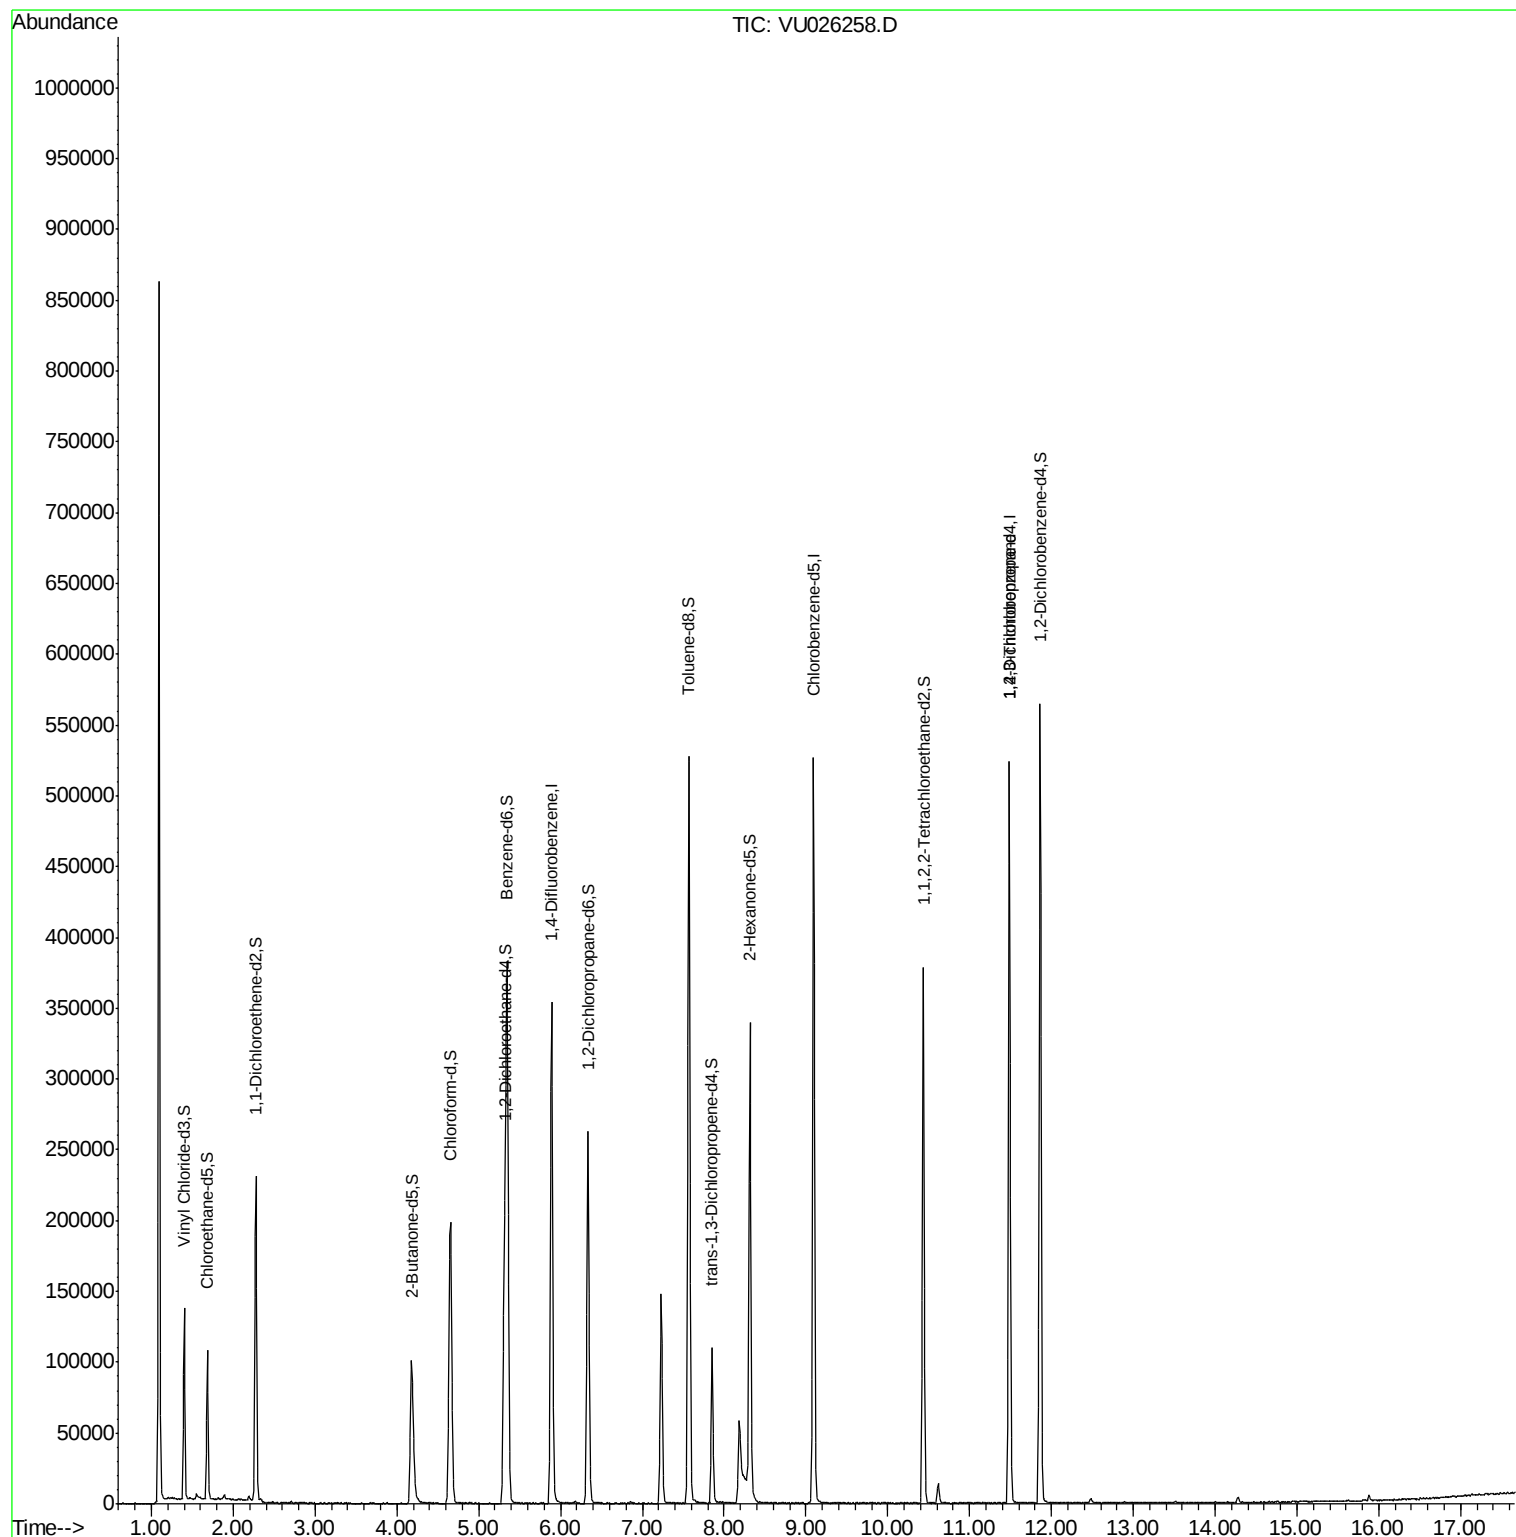

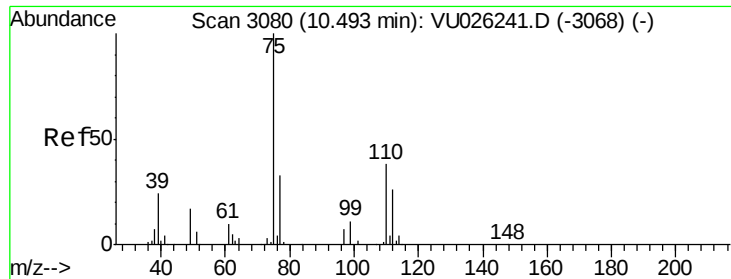

#59

1,2,3-Trichloropropane

Concen: 5.552 ug/L

RT: 11.48 min Scan# 3388

Delta R.T. 0.99 min

Lab File: VU026258.D

Acq: 22 Aug 2018 19:31

Instrument :

MSVOA_U

ClientSampleId :

ETBM9

Tgt Ion: 75 Resp: 14928

Ion Ratio Lower Upper

75 100

77 38.1 25.5 38.3

