

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
 Data File : VU026260.D
 Acq On : 22 Aug 2018 20:18
 Operator : MD/SY
 Sample : J4598-13 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBL3

Quant Time: Aug 23 07:28:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 23 07:27:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	273723	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	267828	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	125607	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	79598	47.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.36%
7) Chloroethane-d5	1.68	69	68338	50.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.27	63	126823	38.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.30%
21) 2-Butanone-d5	4.18	46	150449	112.91	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.91%
24) Chloroform-d	4.65	84	191780	51.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.08%
26) 1,2-Dichloroethane-d4	5.31	65	126991	52.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.88%
32) Benzene-d6	5.35	84	364713	50.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.80%
36) 1,2-Dichloropropane-d6	6.33	67	121364	52.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.50%
41) Toluene-d8	7.57	98	331578	48.42	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.84%
43) trans-1,3-Dichloropropene-	7.85	79	58255	49.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.02%
47) 2-Hexanone-d5	8.31	63	105194	106.99	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.99%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	172669	50.71	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.42%
64) 1,2-Dichlorobenzene-d4	11.86	152	142437	53.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.88%


Target Compounds					Qvalue
37) 1,2-Dichloropropane	6.33	63	13517	6.774 ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU082218\
Data File : VU026260.D
Acq On : 22 Aug 2018 20:18
Operator : MD/SY
Sample : J4598-13 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBL3

Quant Time: Aug 23 07:28:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 23 07:27:18 2018
Response via : Initial Calibration

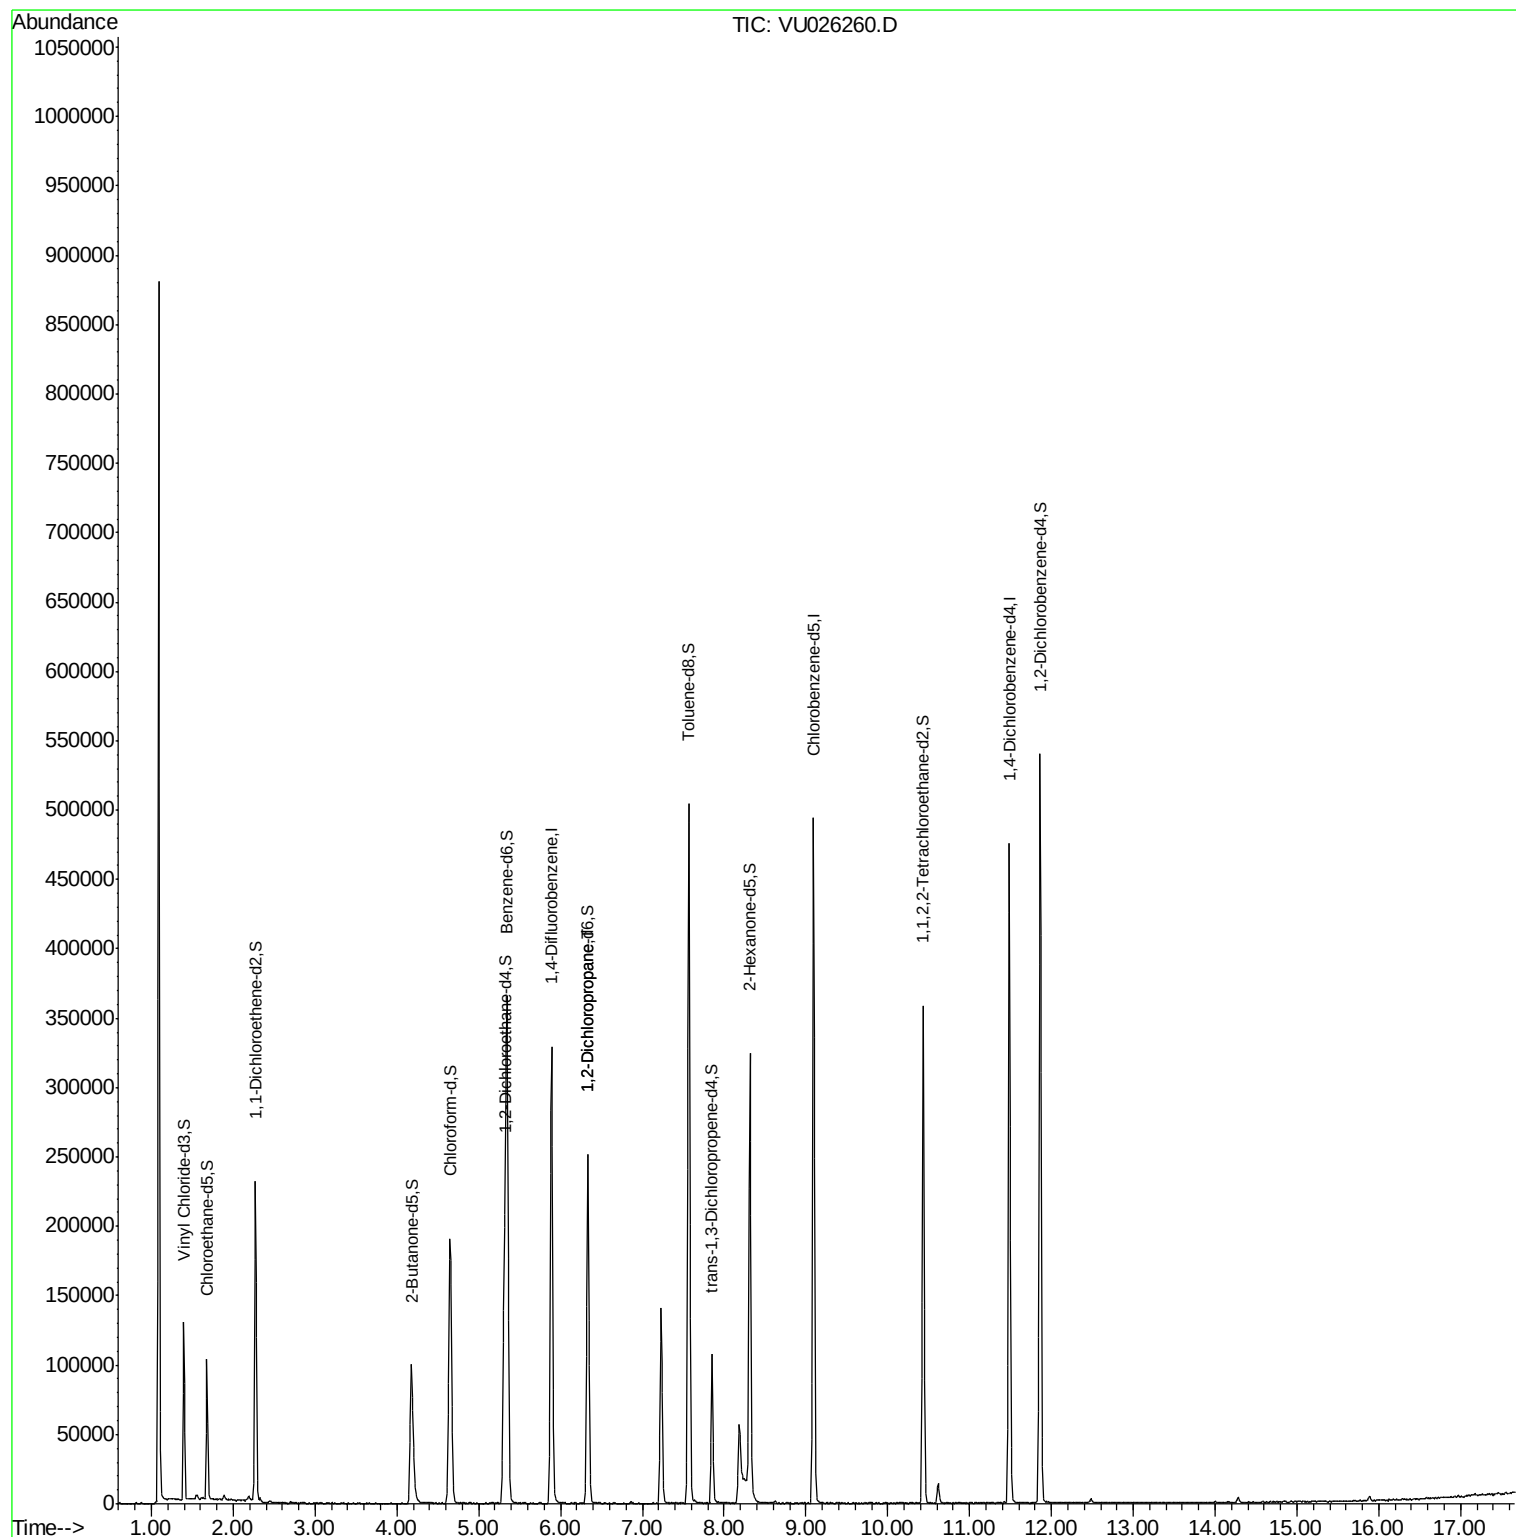

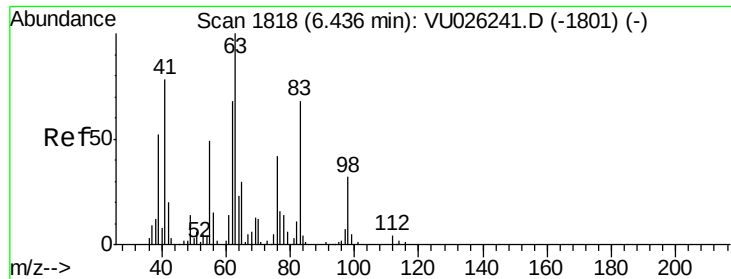

#37
 1,2-Dichloropropane
 Concen: 6.774 ug/L
 RT: 6.33 min Scan# 1786
 Delta R.T. -0.10 min
 Lab File: VU026260.D
 Acq: 22 Aug 2018 20:18

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBL3

Tgt Ion: 63 Resp: 13517
 Ion Ratio Lower Upper
 63 100
 112 0.3 3.4 5.2#

